
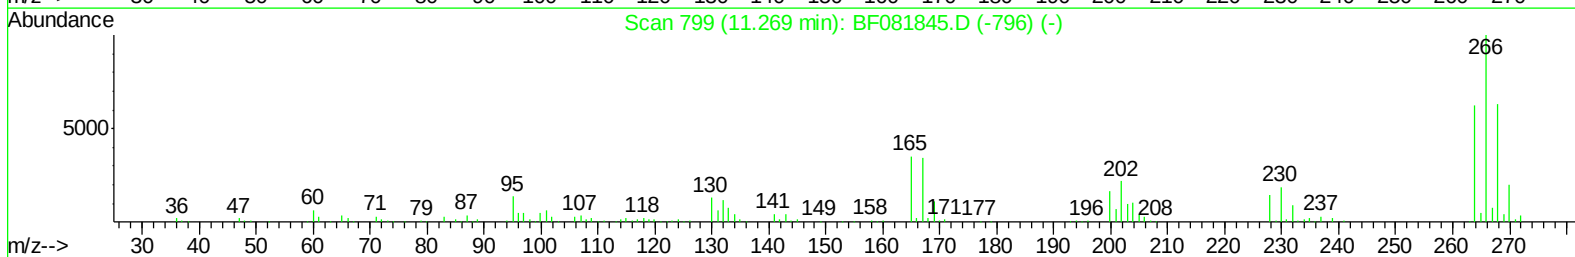
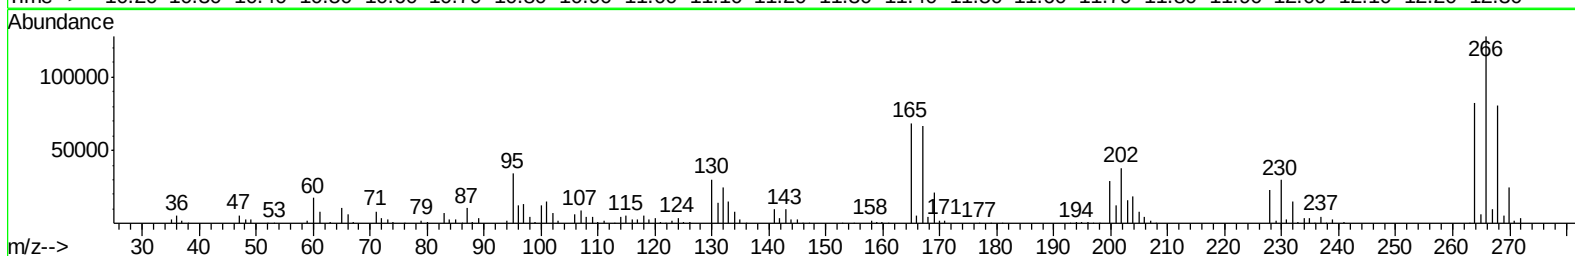


Data Path : Z:\HPCHEM1\BNA_F\Data\BF100515\
 Data File : BF082051.D
 Acq On : 5 Oct 2015 18:26
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 09:22:37 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 05 17:58:12 2015
 Response via : Initial Calibration

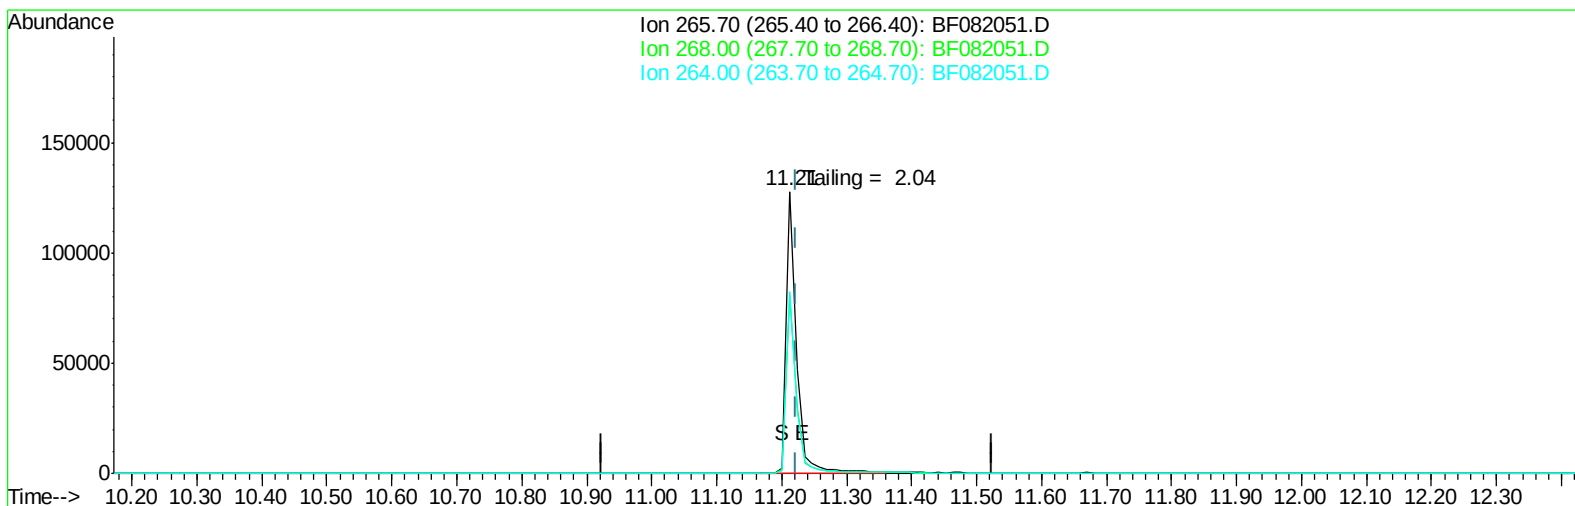

TIC: BF082051.D

(69) Pentachlorophenol (C)




11.212min (-0.011) 0.00ng

response 140814

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.23
264.00	62.70	64.44
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF100515\
Data File : BF082051.D
Acq On : 5 Oct 2015 18:26
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 09:22:37 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 05 17:58:12 2015
Response via : Initial Calibration

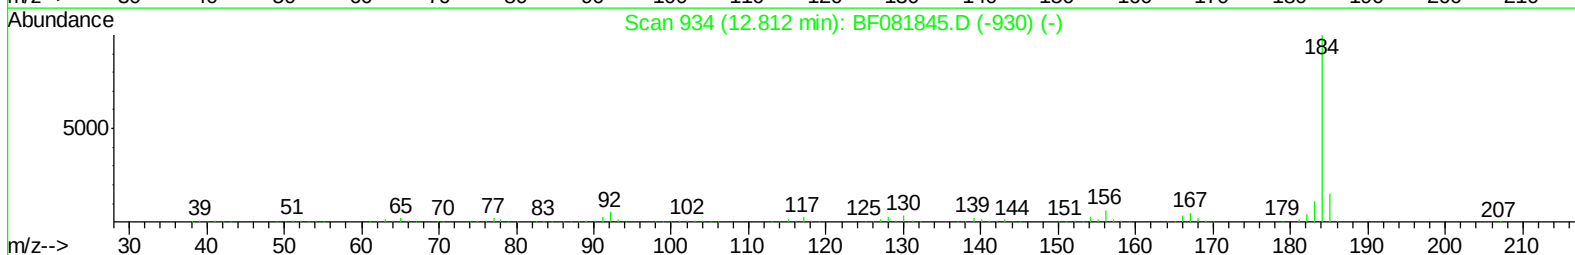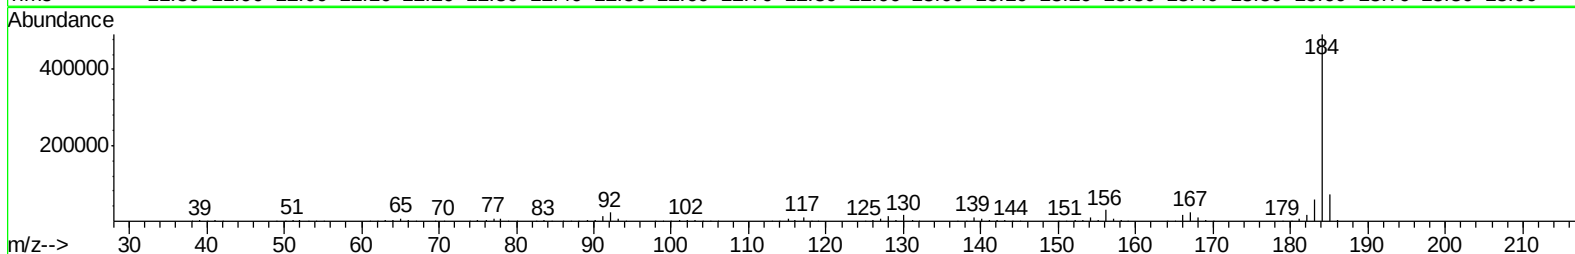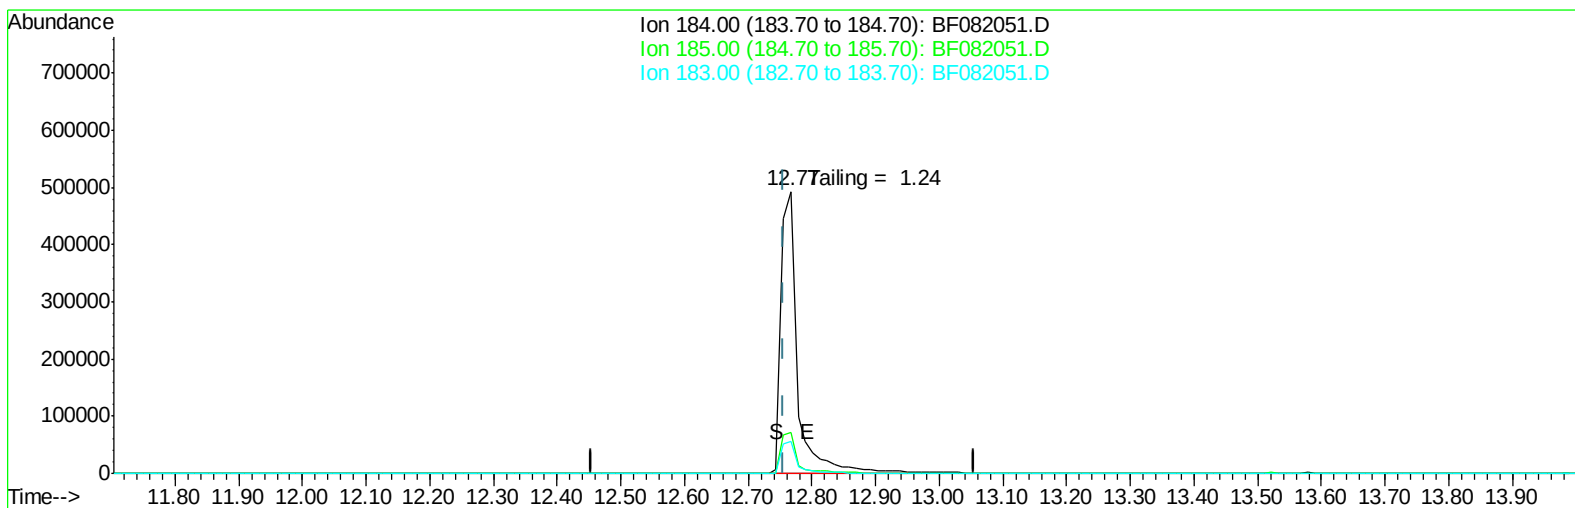

TIC: BF082051.D

(76) Benzidine

12.767min (+0.011) 0.00ng

response 874961

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.49
183.00	9.50	11.56#
0.00	0.00	0.00