


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100515\
Data File : BF082041.D
Acq On : 5 Oct 2015 11:52
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 05 17:58:12 2015

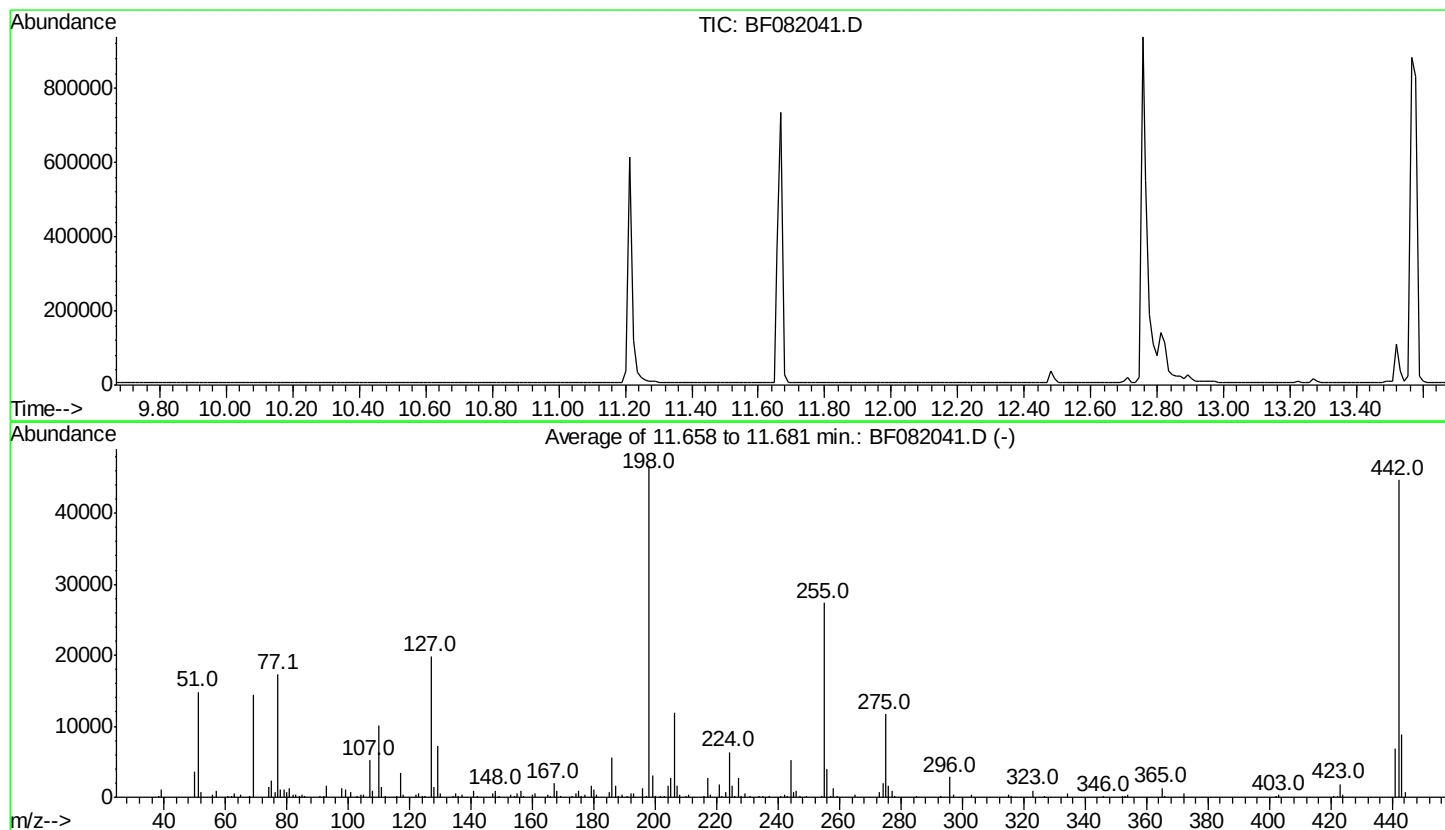

AutoFind: Scans 833, 834, 835; Background Corrected with Scan 829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	14842	PASS
68	69	0.00	2	0.9	134	PASS
69	198	0.00	100	30.8	14365	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.3	19754	PASS
197	198	0.00	2	0.4	188	PASS
198	198	100	100	100.0	46711	PASS
199	198	5	9	6.6	3073	PASS
275	198	10	60	24.9	11638	PASS
365	198	1	100	2.7	1272	PASS
441	442	0.01	24	15.3	6833	PASS
442	198	50	100	95.7	44683	PASS
443	442	15	24	19.6	8761	PASS