


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100515\
 Data File : BF082051.D
 Acq On : 5 Oct 2015 18:26
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 05 17:58:12 2015

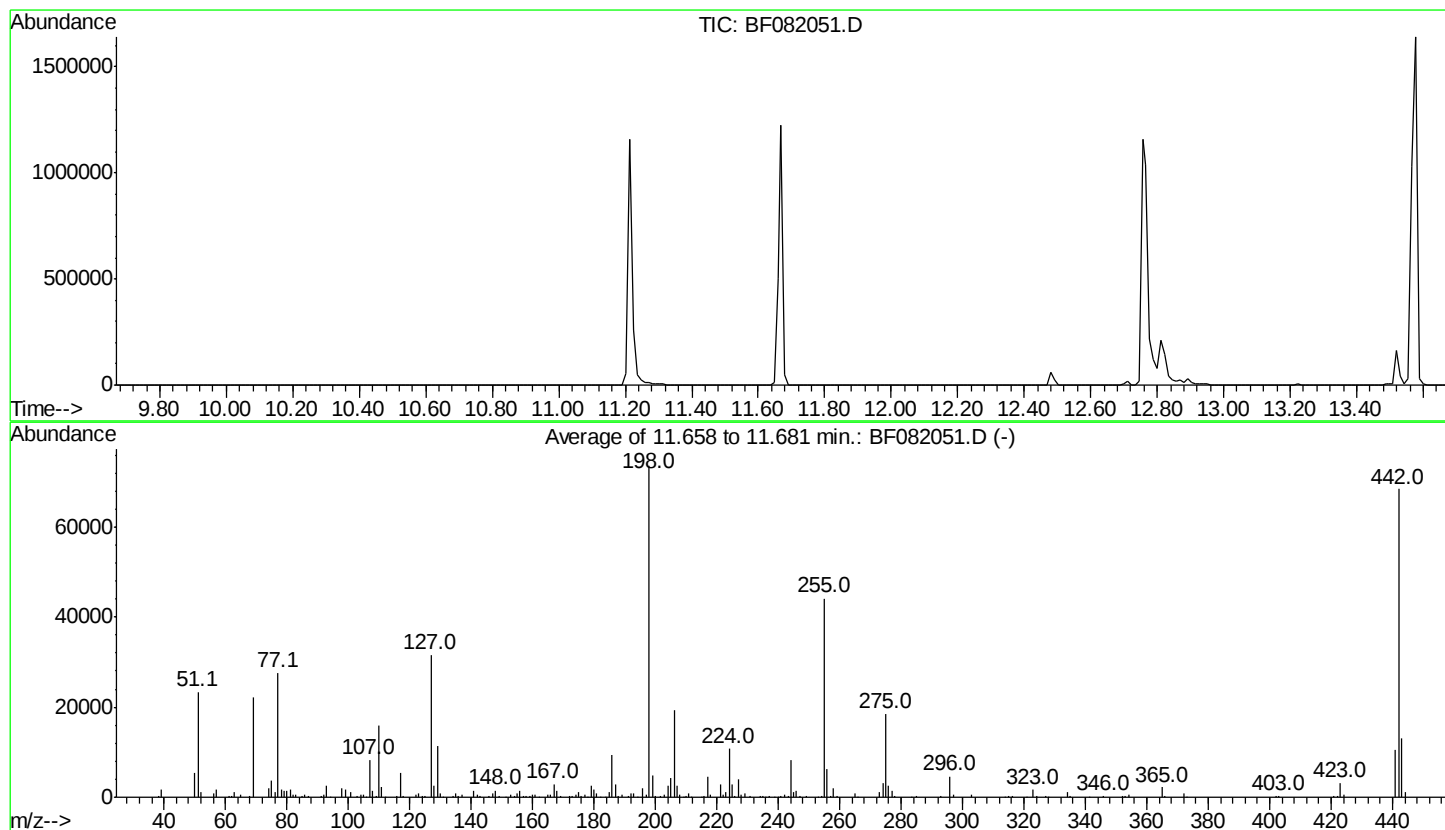

AutoFind: Scans 833, 834, 835; Background Corrected with Scan 829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	23396	PASS
68	69	0.00	2	1.6	360	PASS
69	198	0.00	100	30.3	22288	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.0	31624	PASS
197	198	0.00	2	0.6	454	PASS
198	198	100	100	100.0	73609	PASS
199	198	5	9	6.6	4829	PASS
275	198	10	60	25.2	18536	PASS
365	198	1	100	3.0	2235	PASS
441	442	0.01	24	15.6	10642	PASS
442	198	50	100	92.9	68382	PASS
443	442	15	24	19.3	13174	PASS