
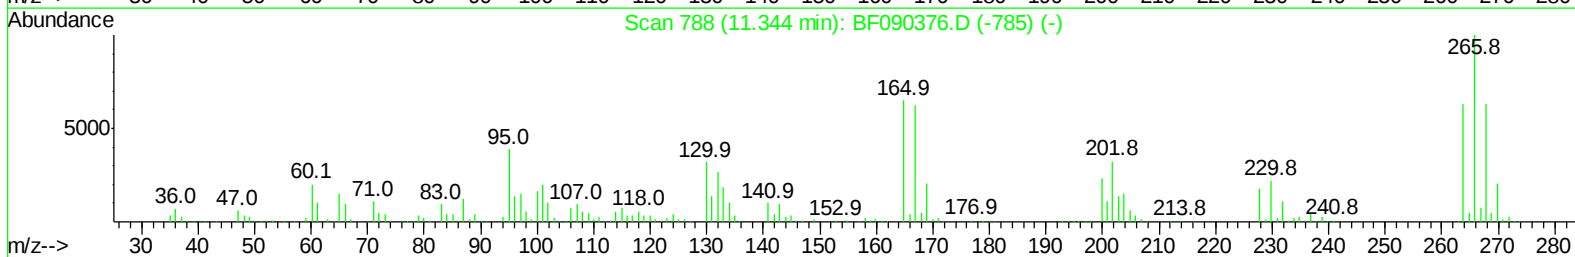
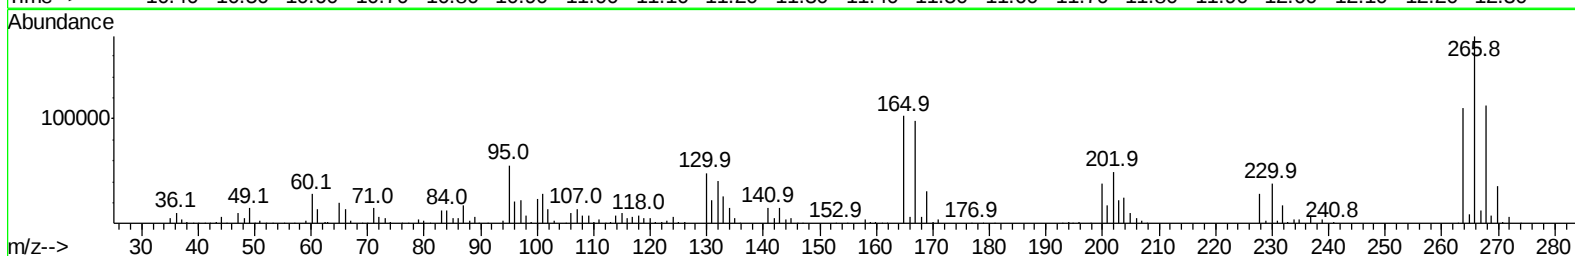


Data Path : Z:\HPCHEM1\BNA F\Data\BF100516\
Data File : BF090371.D
Acq On : 5 Oct 2016 9:19
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 15:11:52 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF100516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 05 14:57:00 2016
Response via : Initial Calibration

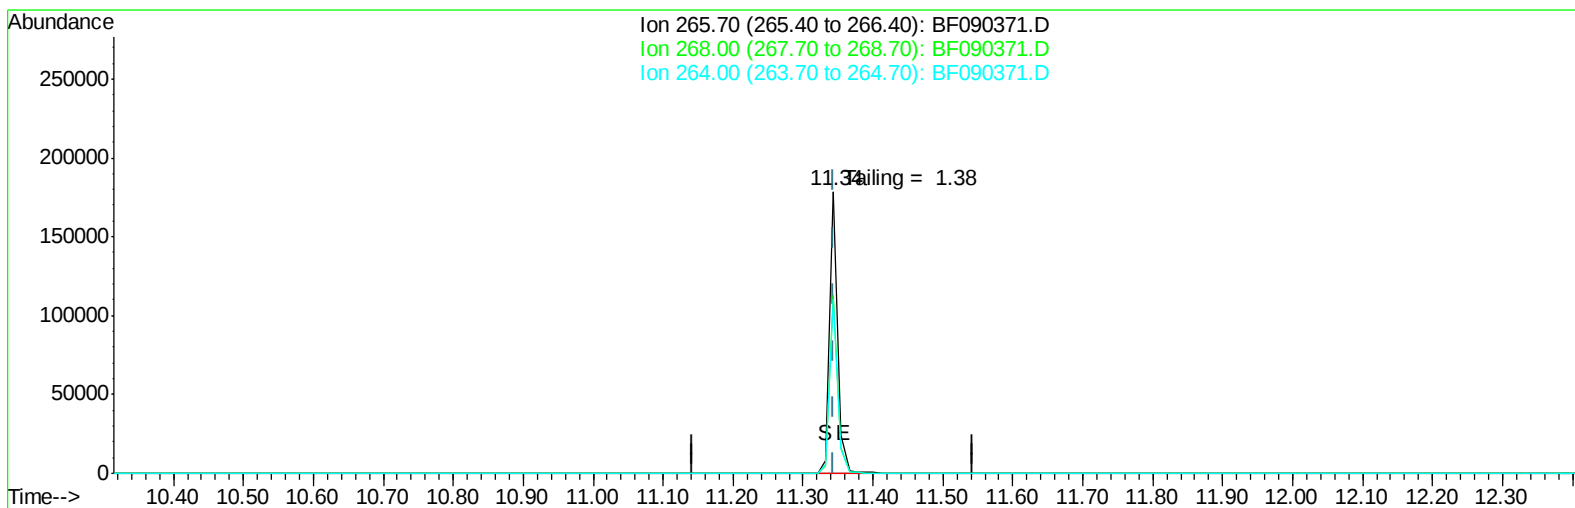

TIC: BF090371.D

(69) Pentachlorophenol (C)

11.343min (-0.000) 0.00ng

response 147639




Ion	Exp%	Act%
265.70	100	100
268.00	63.60	63.34
264.00	64.40	62.02
0.00	0.00	0.00

```

Data Path : Z:\HPCHEM1\BNA F\Data\BF100516\
Data File : BF090371.D
Acq On    : 5 Oct 2016    9:19
Operator  : UM/SJ
Sample    : DFTPP
Misc      :
ALS Vial  : 1    Sample Multiplier: 1

```

Quant Time: Oct 07 15:11:52 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF100516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 05 14:57:00 2016
Response via : Initial Calibration

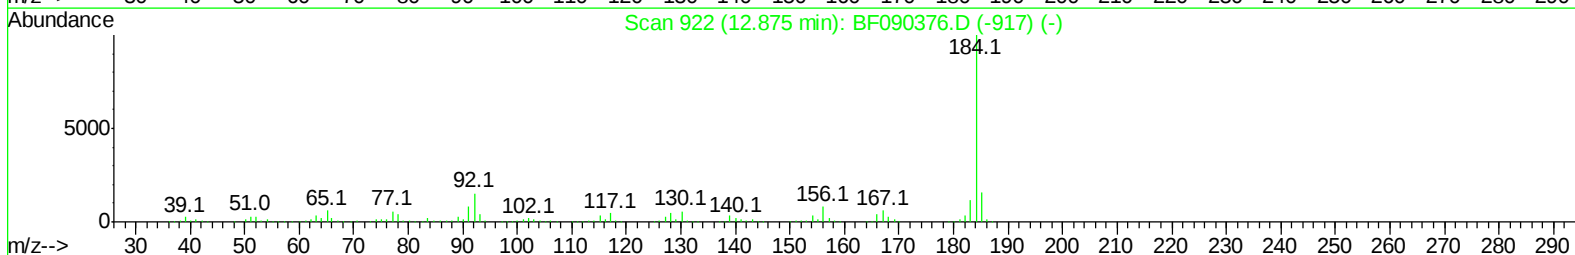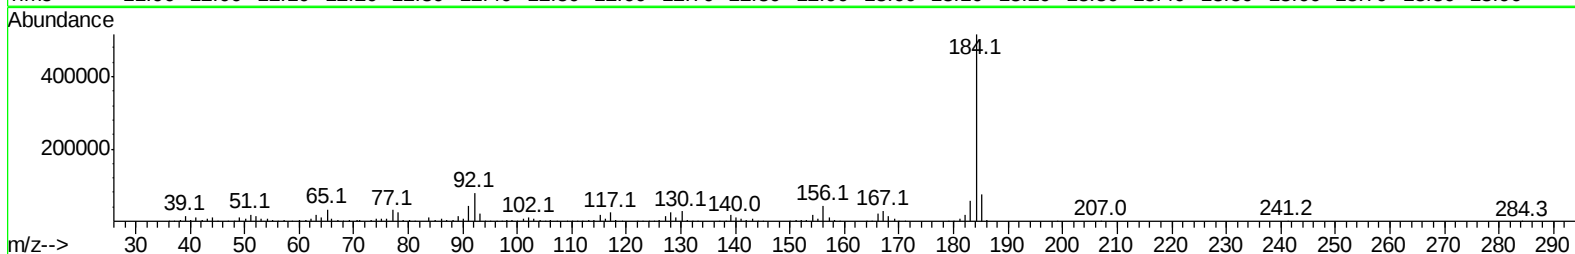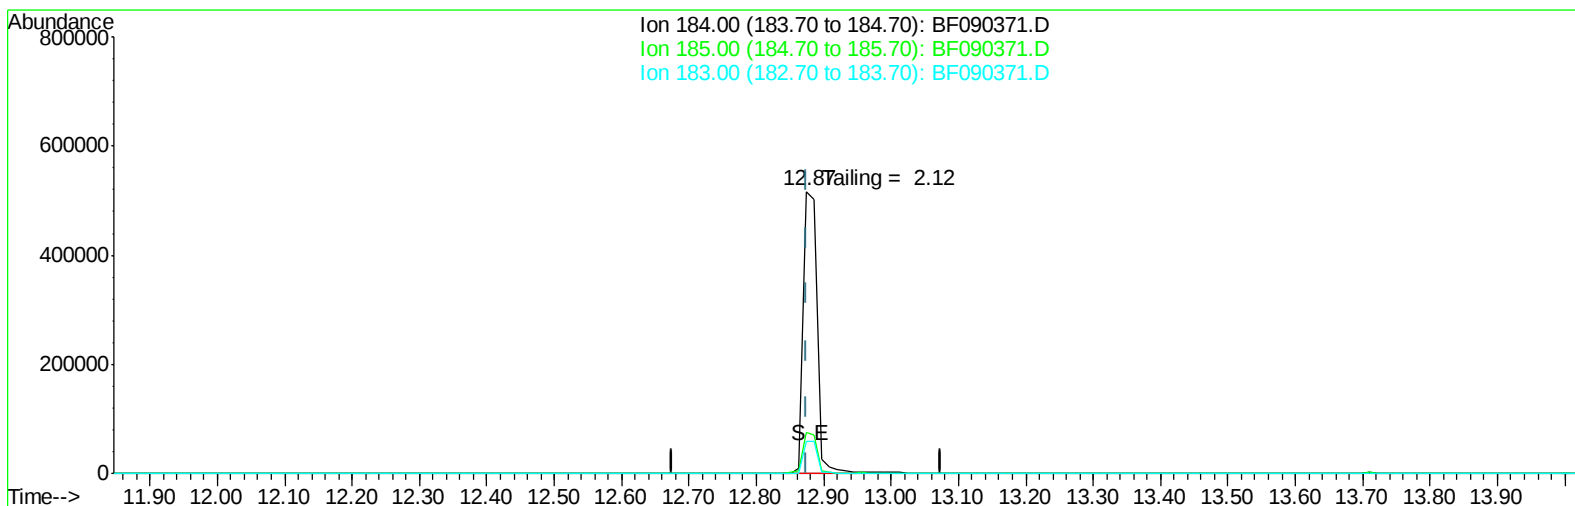

TIC: BF090371.D

(76) Benzidine

12.875min (-0.000) 81977.28ng

response 747950

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.67
183.00	12.00	11.31
0.00	0.00	0.00