
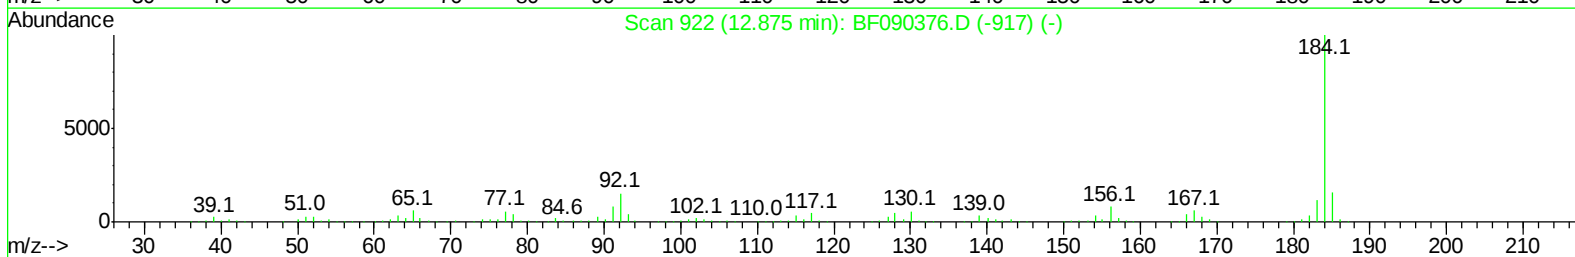
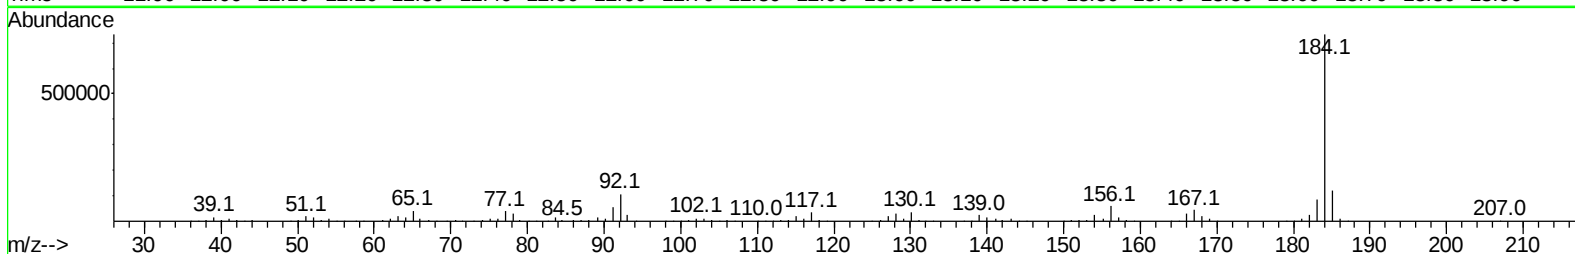


Data Path : Z:\HPCHEM1\BNA F\Data\BF100516\
Data File : BF090381.D
Acq On : 5 Oct 2016 15:08
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 15:18:21 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF100516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 05 14:57:00 2016
Response via : Initial Calibration

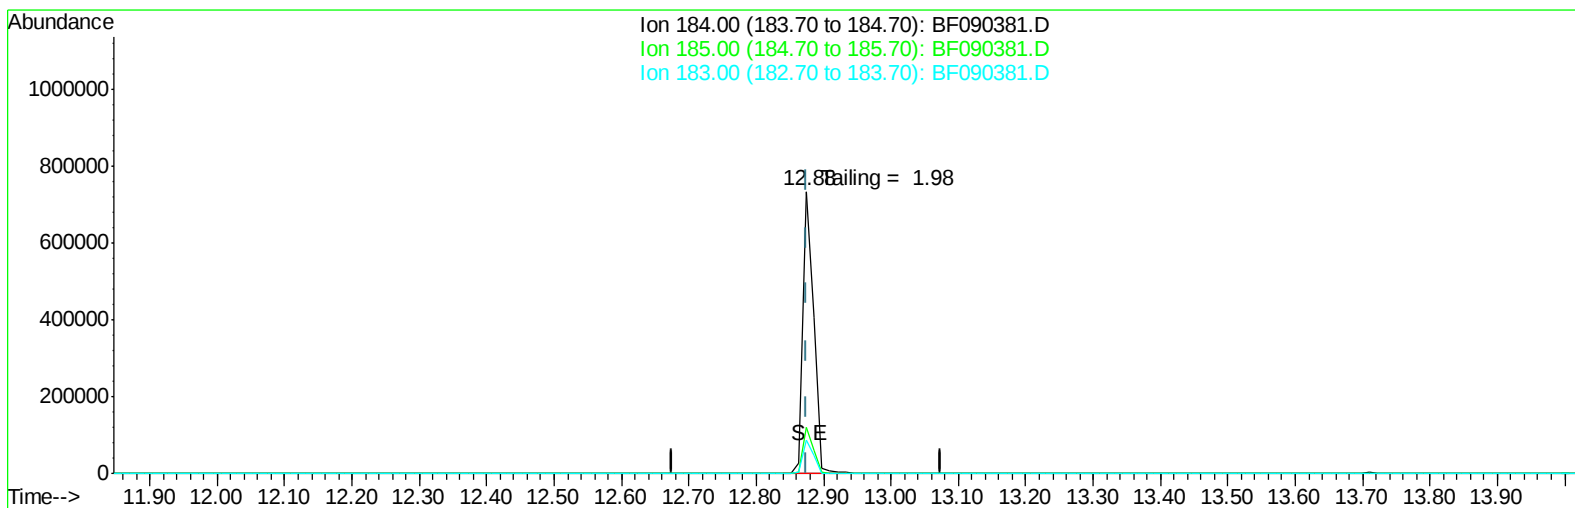

TIC: BF090381.D

(76) Benzidine




12.875min (+0.000) 64423.97ng

response 821559

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	16.50
183.00	12.00	11.76
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF100516\
Data File : BF090381.D
Acq On : 5 Oct 2016 15:08
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 15:18:21 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF100516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 05 14:57:00 2016
Response via : Initial Calibration

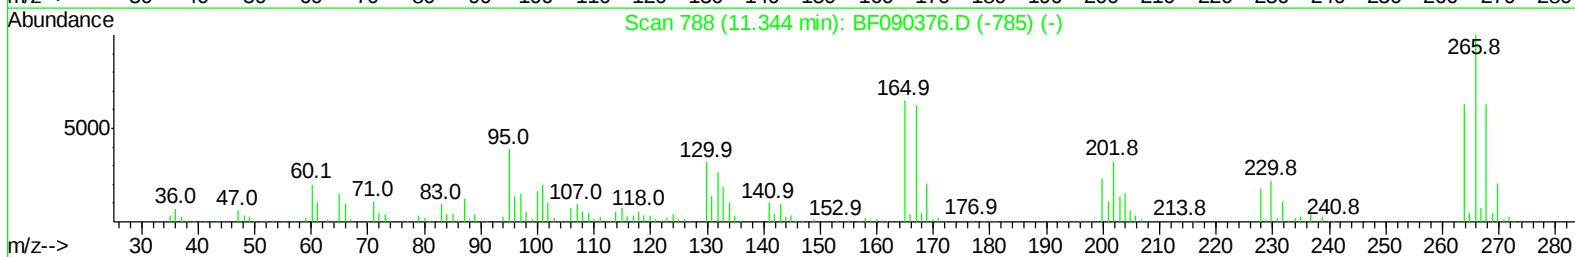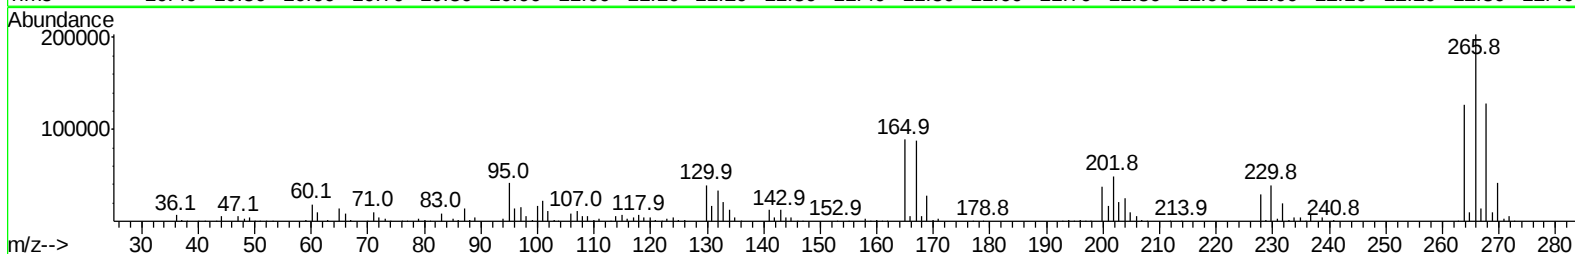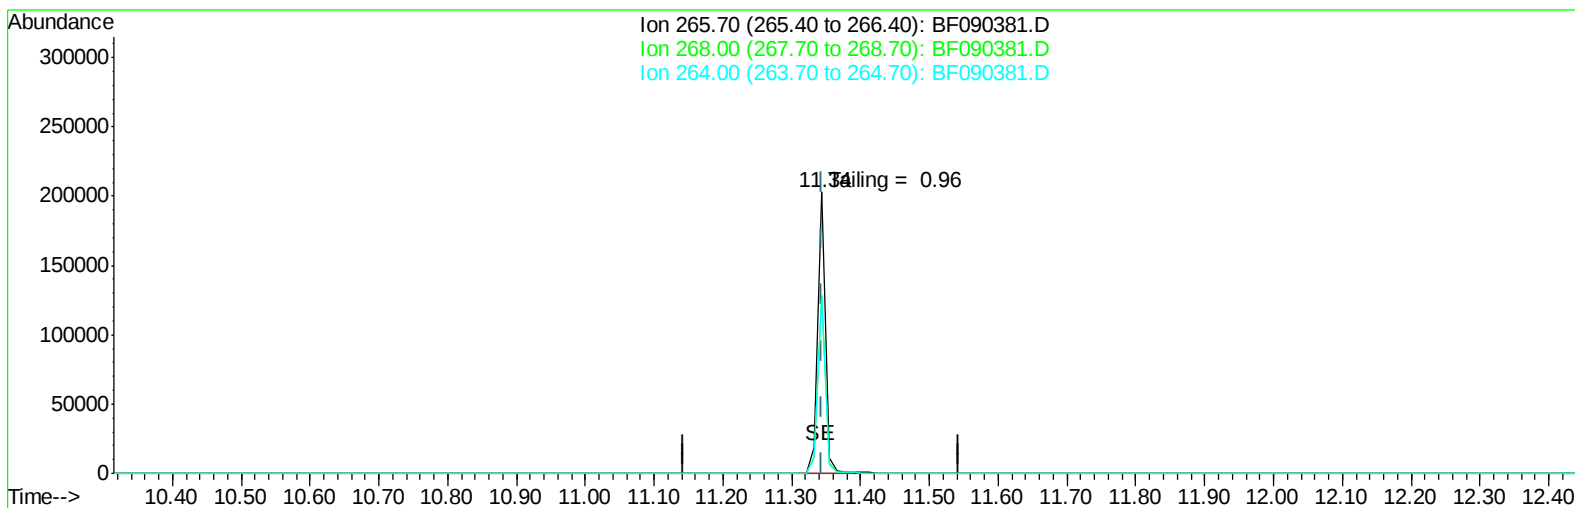

TIC: BF090381.D

(69) Pentachlorophenol (C)

11.344min (+0.000) 56188.82ng

response 163571

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	63.20
264.00	64.40	62.21
0.00	0.00	0.00