
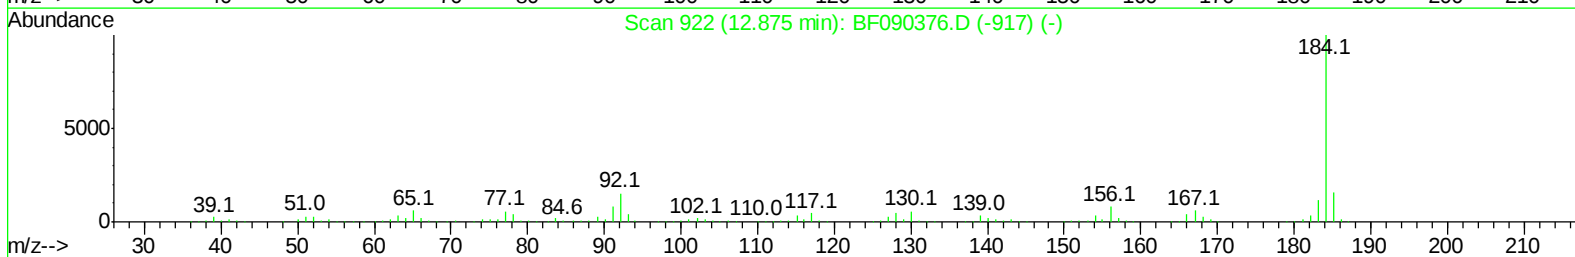
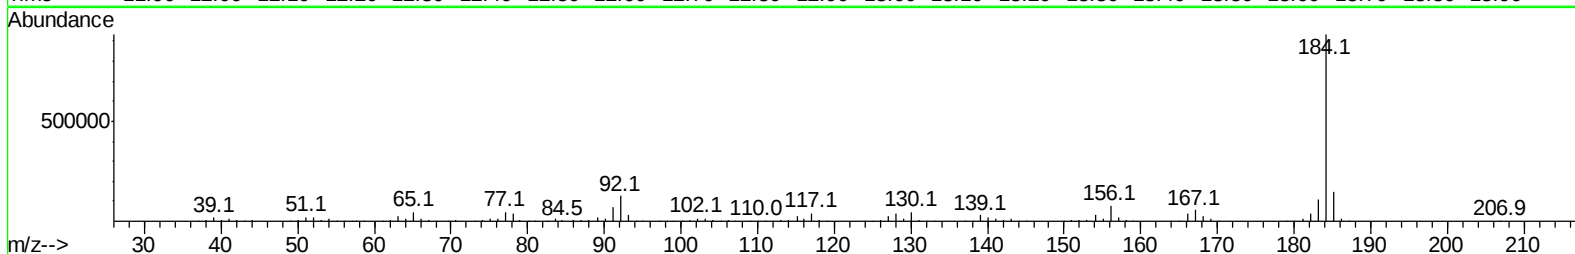


Data Path : Z:\HPCHEM1\BNA F\Data\BF100516\  
Data File : BF090405.D  
Acq On : 6 Oct 2016 2:57  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 15:20:54 2016  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF100516.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Oct 05 14:57:00 2016  
Response via : Initial Calibration

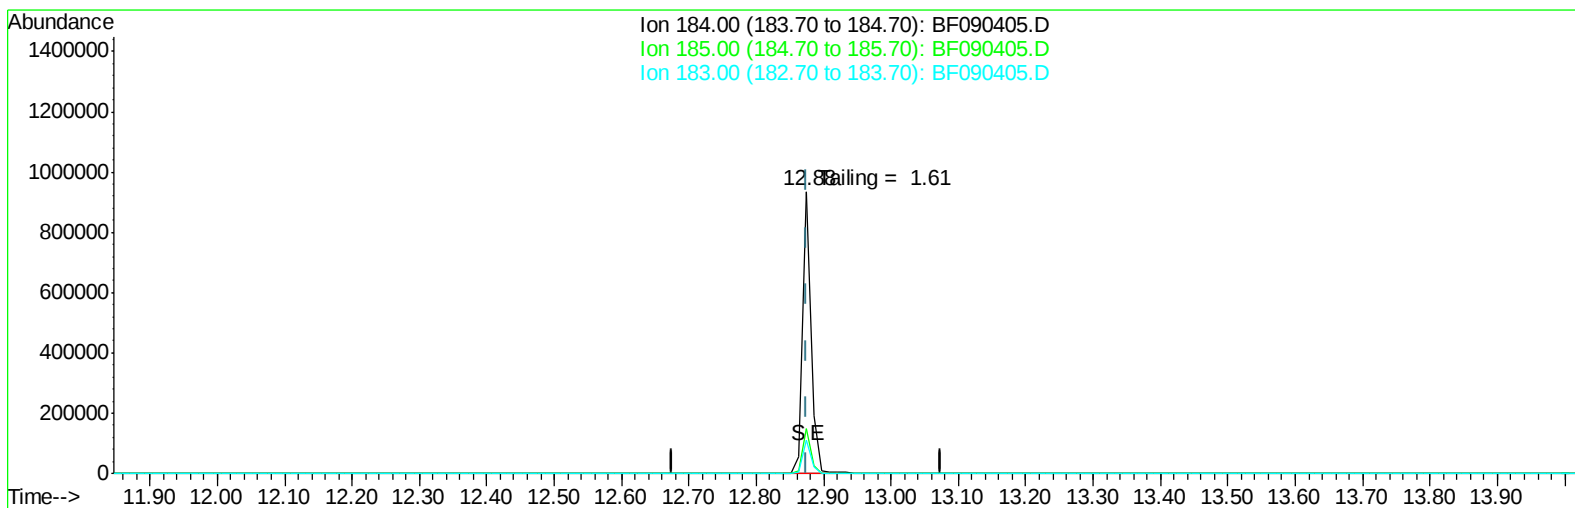

TIC: BF090405.D

(76) Benzidine




12.875min (-0.000) 44696.49ng m

response 821486

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.80 | 16.01 |
| 183.00 | 12.00 | 11.71 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA F\Data\BF100516\  
Data File : BF090405.D  
Acq On : 6 Oct 2016 2:57  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 15:20:54 2016  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF100516.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Oct 05 14:57:00 2016  
Response via : Initial Calibration

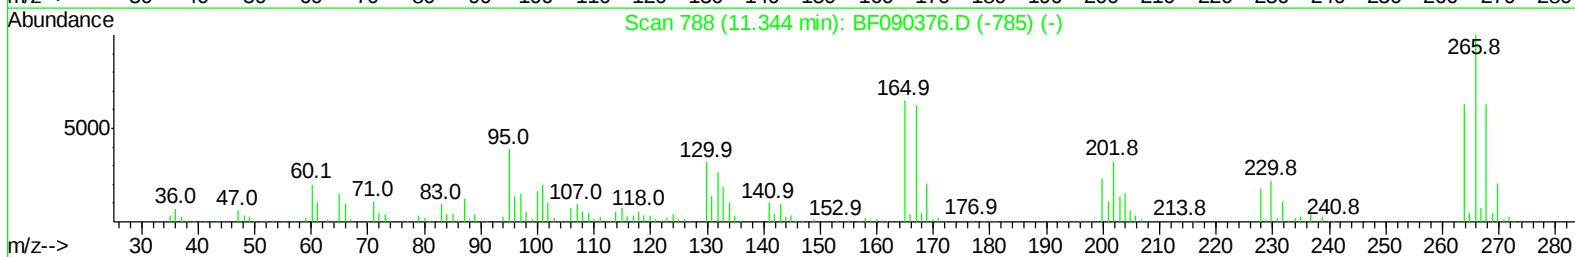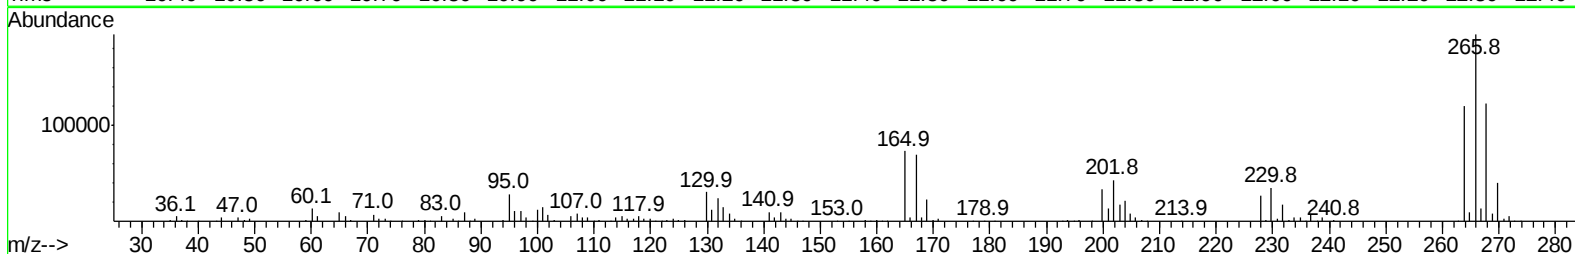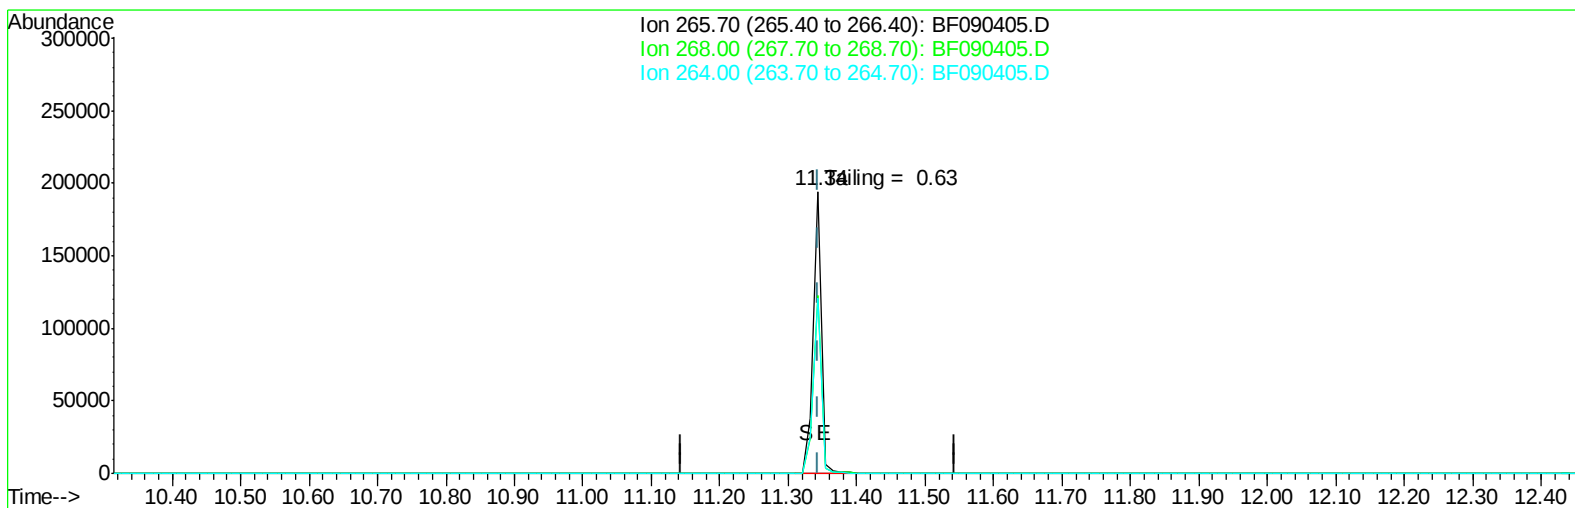

TIC: BF090405.D

(69) Pentachlorophenol (C)

11.343min (-0.000) 27067.97ng

response 166741

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.60 | 63.24 |
| 264.00 | 64.40 | 62.06 |
| 0.00   | 0.00  | 0.00  |