

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100516\
 Data File : BF090414.D
 Acq On : 6 Oct 2016 7:06
 Operator : UM/SJ
 Sample : PB93730BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB93730BL

Quant Time: Oct 06 07:52:18 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF100516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 05 14:57:00 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.00	152	263733	20.00	ng	0.00
21) Naphthalene-d8	8.29	136	1106958	20.00	ng	0.00
38) Acenaphthene-d10	10.05	164	573083	20.00	ng	0.00
63) Phenanthrene-d10	11.54	188	832269	20.00	ng	-0.01
75) Chrysene-d12	14.19	240	677991	20.00	ng	-0.01
86) Perylene-d12	15.69	264	453630	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	1822607	103.14	ng	0.01
7) Phenol-d6	6.62	99	2253303	97.36	ng	0.00
23) Nitrobenzene-d5	7.56	82	1468194	64.52	ng	-0.01
41) 2,4,6-Tribromophenol	10.84	330	505223	108.42	ng	-0.01
44) 2-Fluorobiphenyl	9.37	172	2297065	66.78	ng	-0.01
78) Terphenyl-d14	13.14	244	2666293	88.41	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100516\
Data File : BF090414.D
Acq On : 6 Oct 2016 7:06
Operator : UM/SJ
Sample : PB93730BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB93730BL

Quant Time: Oct 06 07:52:18 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF100516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 05 14:57:00 2016
Response via : Initial Calibration

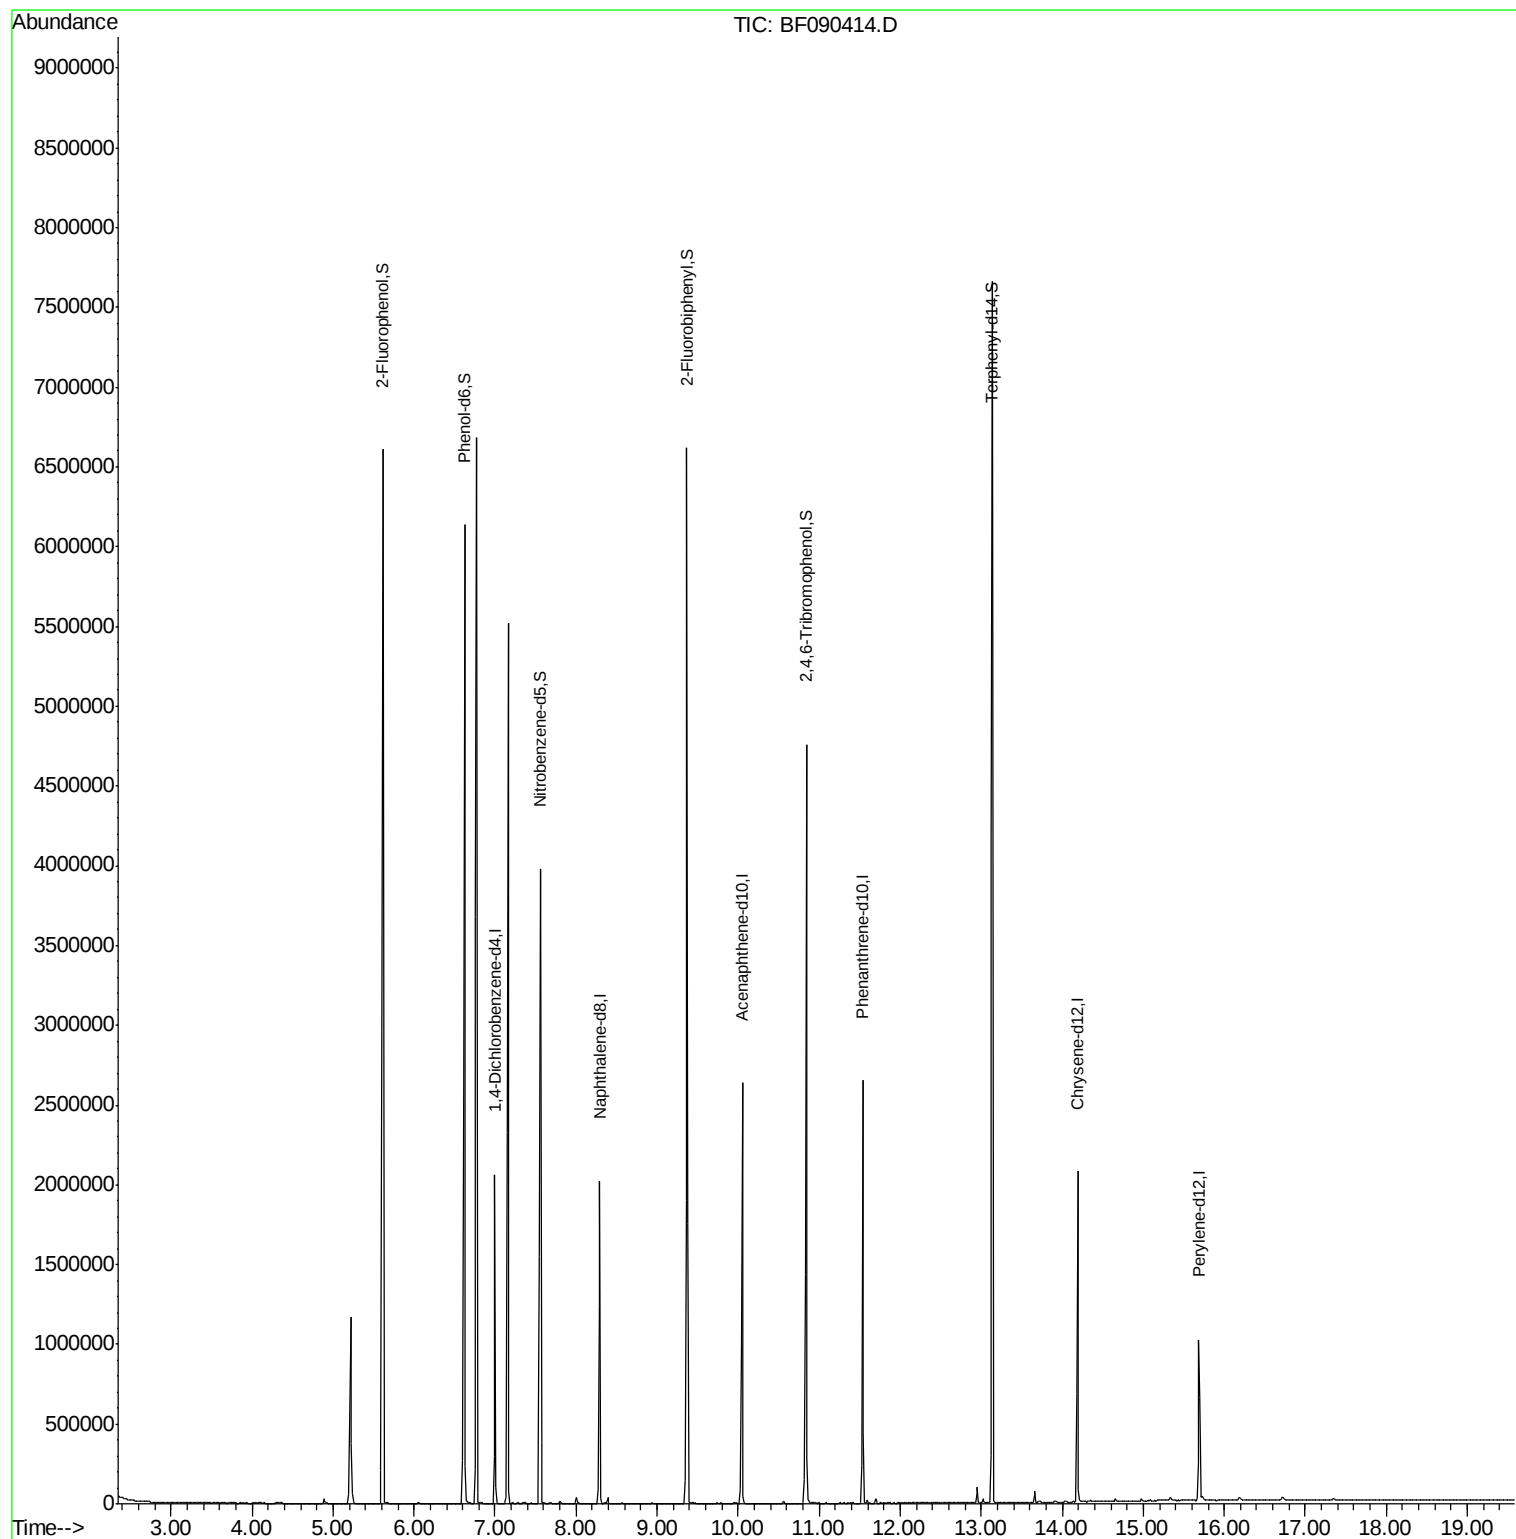

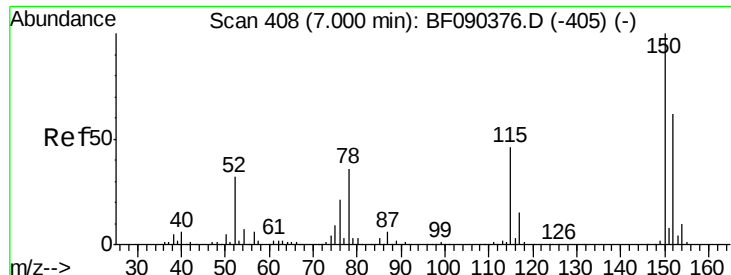

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.00 min Scan# 408

Delta R.T. -0.00 min

Lab File: BF090414.D

Acq: 6 Oct 2016 7:06

Instrument :

BNA_F

ClientSampleId :

PB93730BL


Tot Ion:152 Resp: 263733

Ion Ratio Lower Upper

152 100

150 158.1 124.6 186.8




115 66.4 46.2 69.4

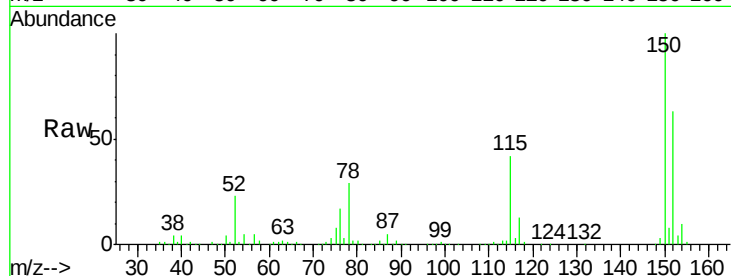

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

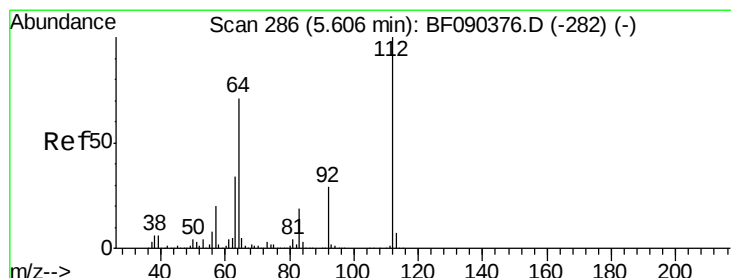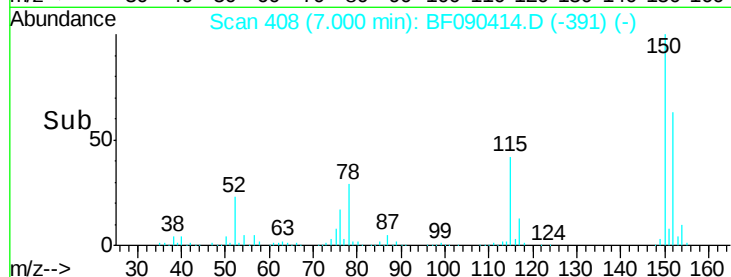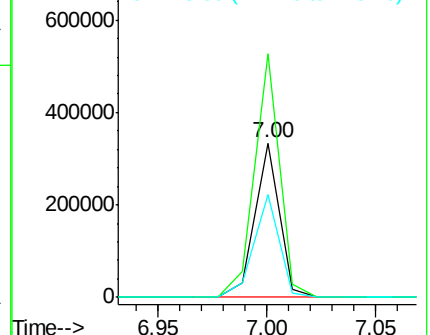

#5

2-Fluorophenol

Concen: 103.14 ng

RT: 5.62 min Scan# 287

Delta R.T. 0.01 min

Lab File: BF090414.D

Acq: 6 Oct 2016 7:06


Tgt Ion:112 Resp: 1822607

Ion Ratio Lower Upper

112 100

64 69.2 57.9 86.9



63 33.6 29.6 44.4

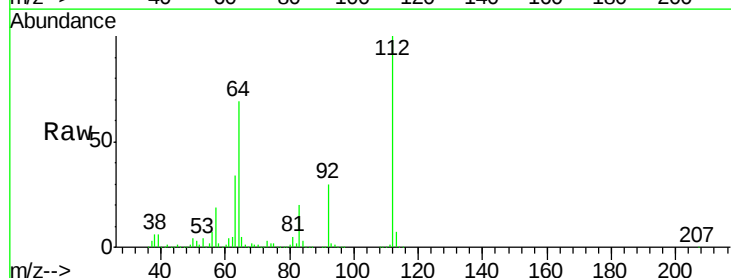

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

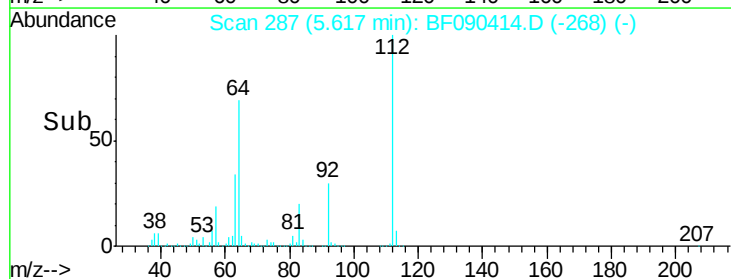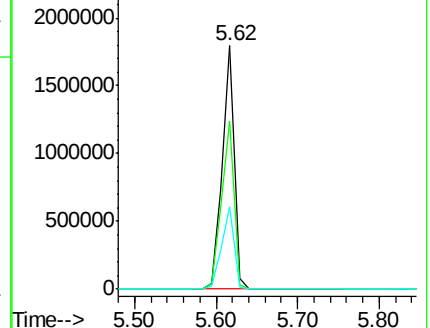



#7

Phenol-d6

Concen: 97.36 ng

RT: 6.62 min Scan# 375

Delta R.T. -0.00 min

Lab File: BF090414.D

Acq: 6 Oct 2016 7:06

Instrument :





BNA_F

ClientSampleId :

PB93730BL

Tot Ion: 99 Resp: 2253303

Ion	Ratio	Lower	Upper
99	100		
42	17.4	20.0	30.0#
71	34.2	27.9	41.9

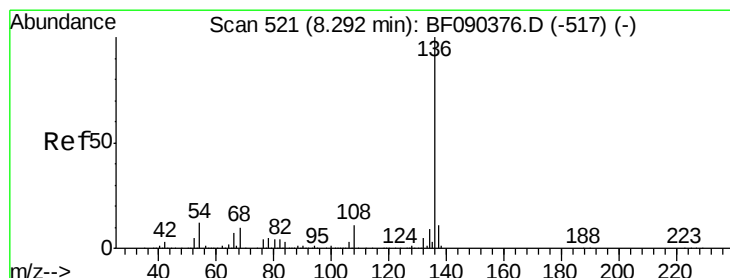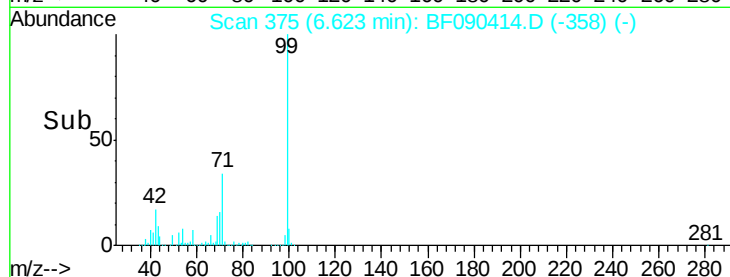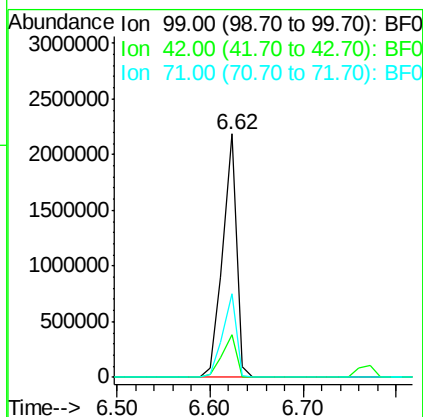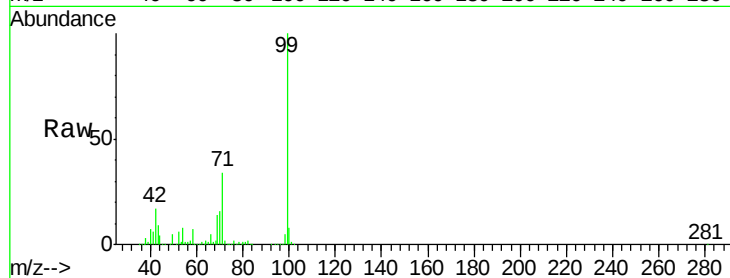

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.29 min Scan# 521




Delta R.T. -0.00 min


Lab File: BF090414.D

Acq: 6 Oct 2016 7:06

Tgt Ion: 136 Resp: 1106958

Ion	Ratio	Lower	Upper
136	100		
137	10.9	9.0	13.6
54	8.3	6.6	10.0
68	7.3	5.0	7.6

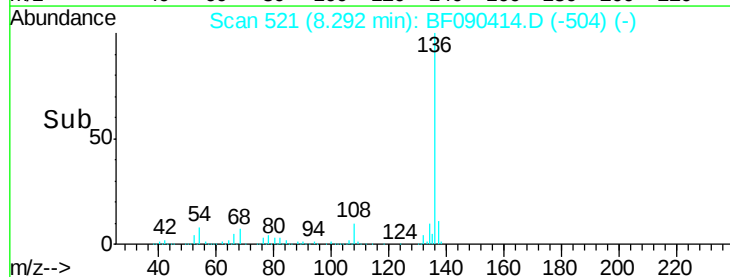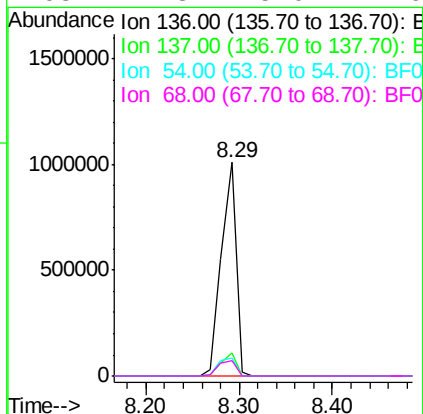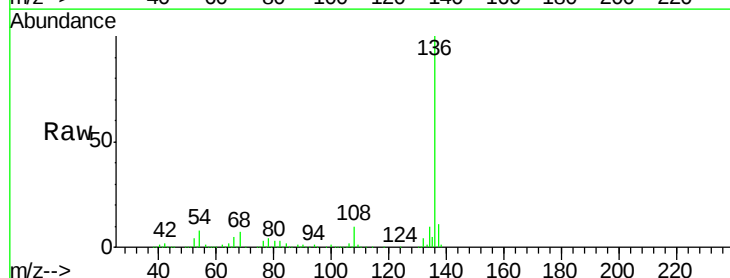


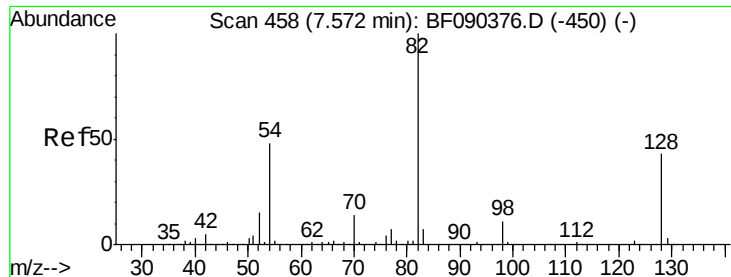




#23
 Nitrobenzene-d5
 Concen: 64.52 ng
 RT: 7.56 min Scan# 457
 Delta R.T. -0.01 min
 Lab File: BF090414.D
 Acq: 6 Oct 2016 7:06

Instrument :
 BNA_F
 ClientSampleID :
 PB93730BL

Tot Ion: 82 Resp: 1468194
 Ion Ratio Lower Upper
 82 100
 128 39.9 40.0 60.0#
 54 50.6 42.6 64.0

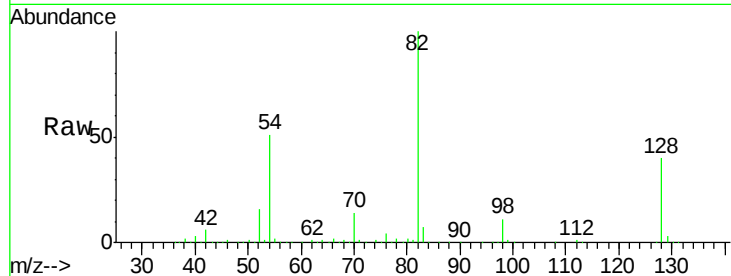


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

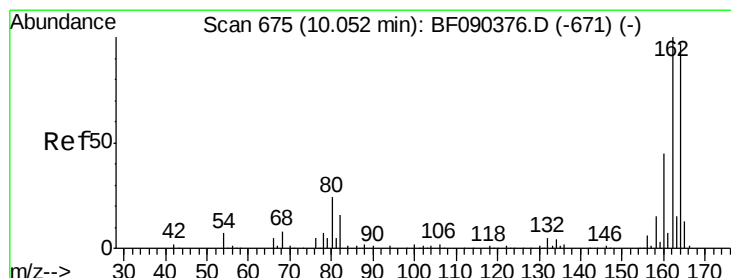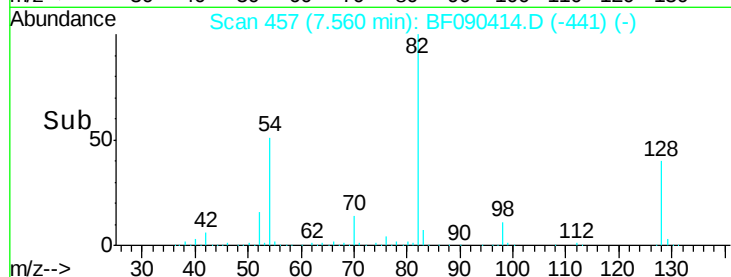
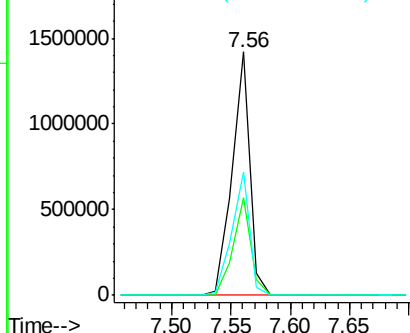



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.05 min Scan# 675
 Delta R.T. -0.00 min
 Lab File: BF090414.D
 Acq: 6 Oct 2016 7:06

Tgt Ion:164 Resp: 573083
 Ion Ratio Lower Upper
 164 100
 162 104.2 80.1 120.1
 160 47.1 36.3 54.5

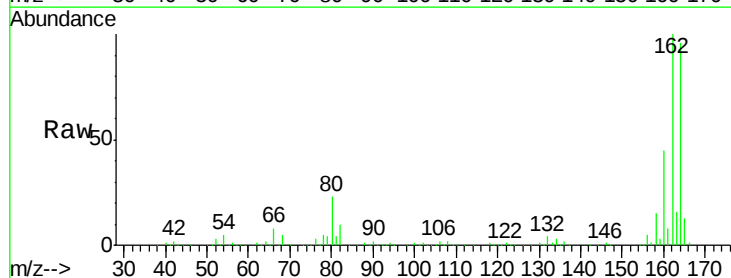

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E



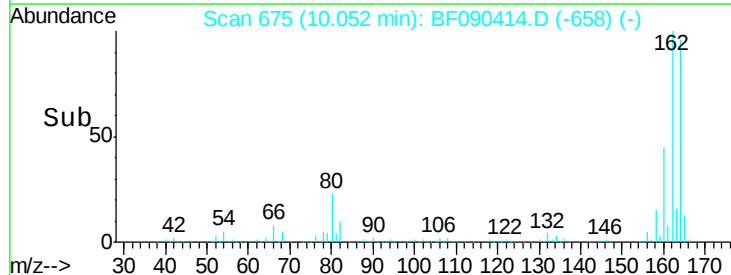
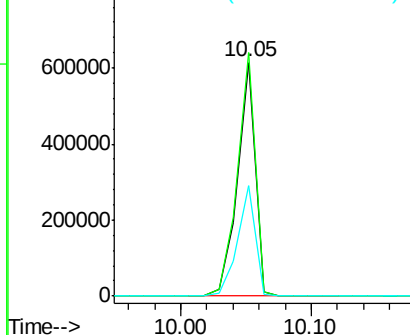


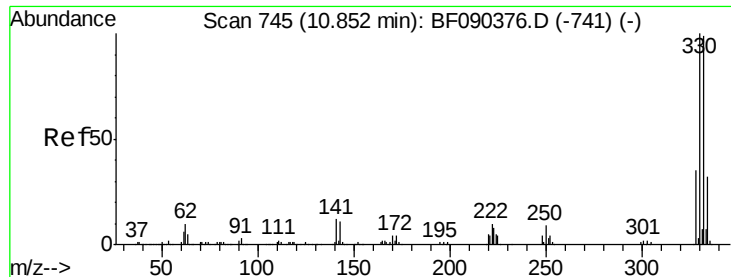

#41
 2,4,6-Tribromophenol
 Concen: 108.42 ng
 RT: 10.84 min Scan# 744
 Delta R.T. -0.01 min
 Lab File: BF090414.D
 Acq: 6 Oct 2016 7:06




Instrument :
 BNA_F
 ClientSampleId :
 PB93730BL


Tot Ion	Ratio	Lower	Upper
330	100		
332	94.8	75.4	113.0
141	44.0	26.9	40.3

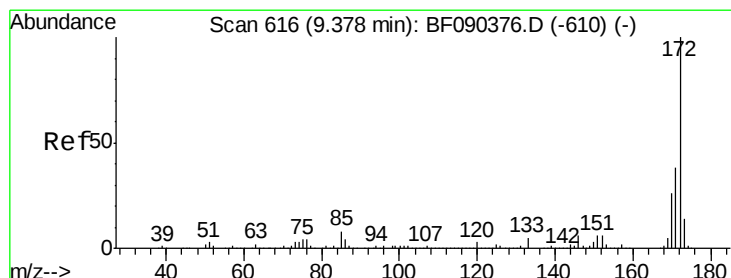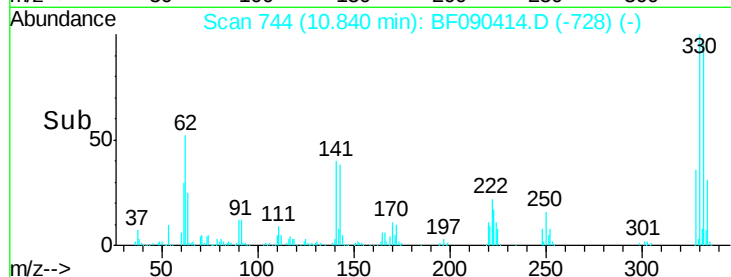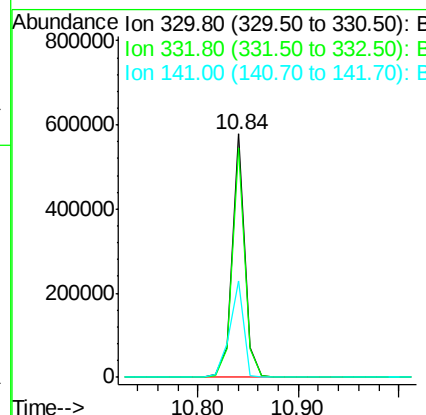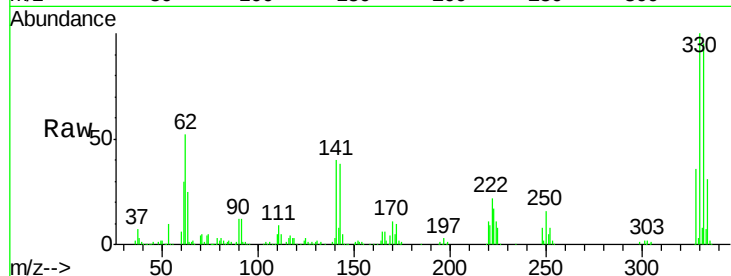

#44
 2-Fluorobiphenyl
 Concen: 66.78 ng
 RT: 9.37 min Scan# 615
 Delta R.T. -0.01 min
 Lab File: BF090414.D
 Acq: 6 Oct 2016 7:06

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.5	31.8	47.8
170	25.6	21.7	32.5

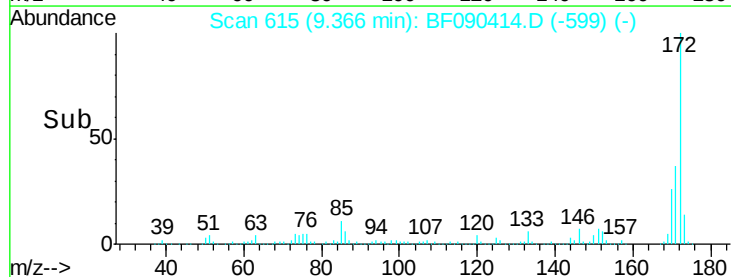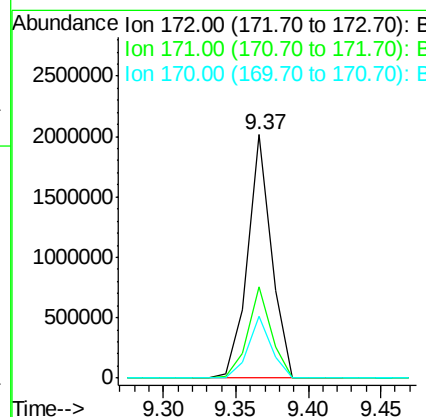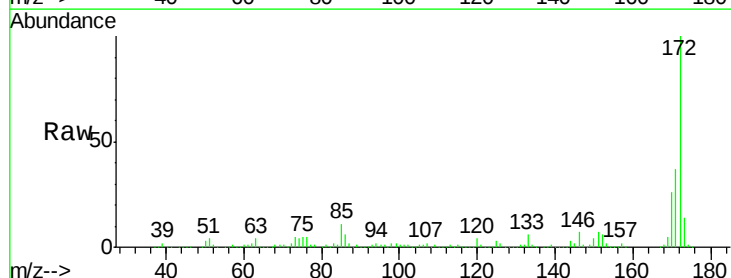


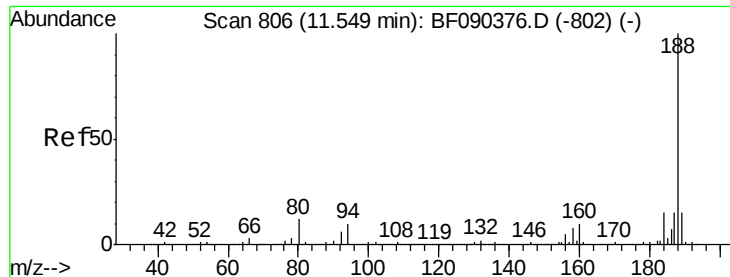




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.54 min Scan# 805
Delta R.T. -0.01 min
Lab File: BF090414.D
Acq: 6 Oct 2016 7:06

Instrument :
BNA_F
ClientSampleId :
PB93730BL

Tot Ion:188 Resp: 832269
Ion Ratio Lower Upper
188 100
94 15.8 8.2 12.2#
80 19.1 8.8 13.2#

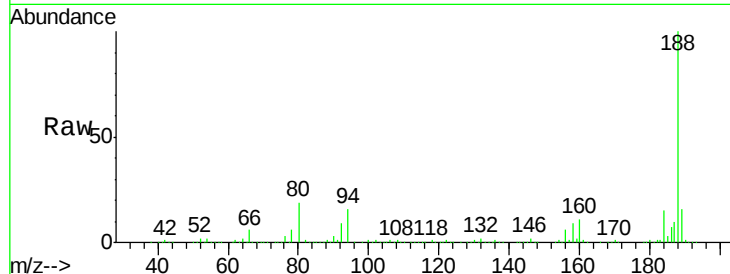


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

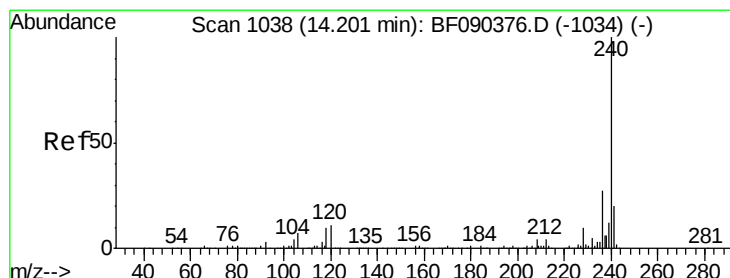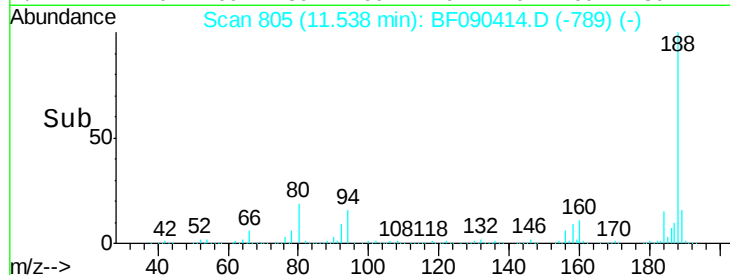
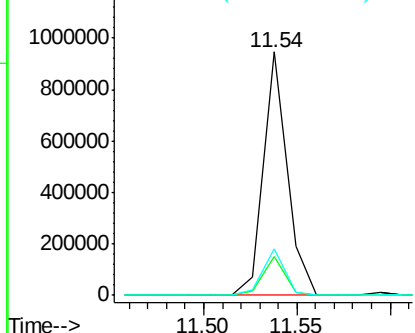



#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.19 min Scan# 1037
Delta R.T. -0.01 min
Lab File: BF090414.D
Acq: 6 Oct 2016 7:06

Tgt Ion:240 Resp: 677991
Ion Ratio Lower Upper
240 100
120 12.1 8.6 13.0
236 27.0 21.6 32.4

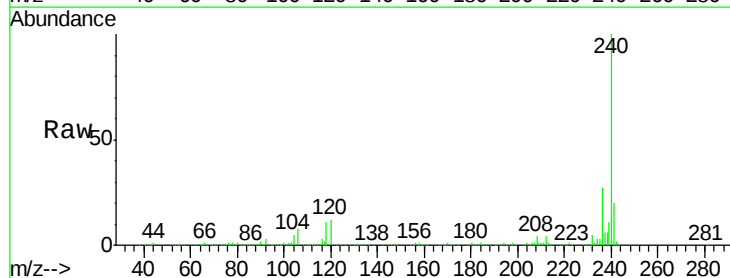

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

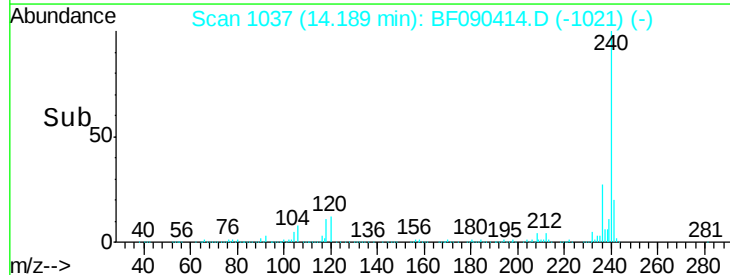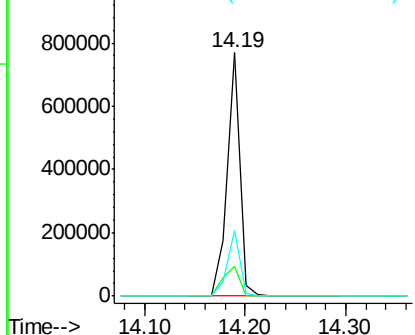

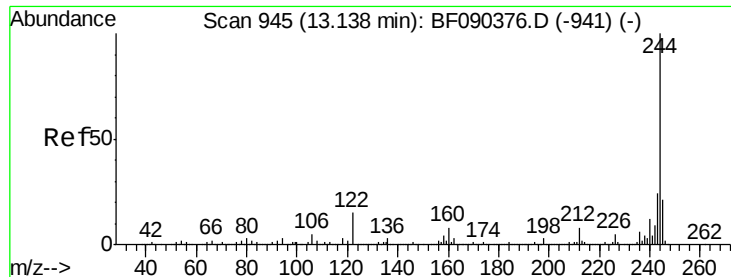

#78

Terphenyl-d14

Concen: 88.41 ng

RT: 13.14 min Scan# 945

Delta R.T. -0.00 min

Lab File: BF090414.D

Acq: 6 Oct 2016 7:06

Instrument :

BNA_F

ClientSampleId :

PB93730BL


Tot Ion:244 Resp: 2666293

Ion Ratio Lower Upper

244 100

212 7.4 6.8 10.2




122 11.0 13.3 19.9#

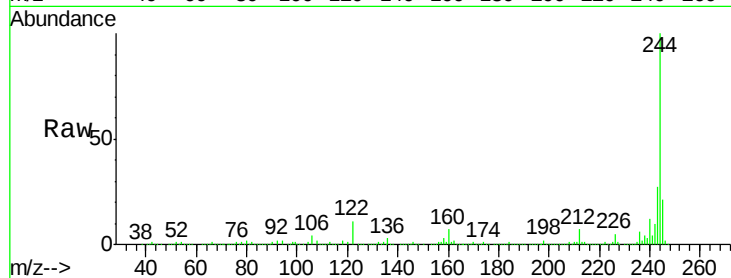

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

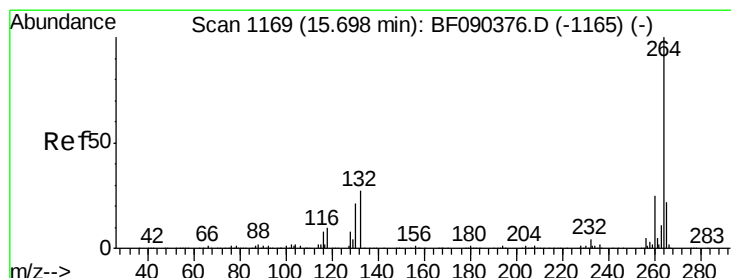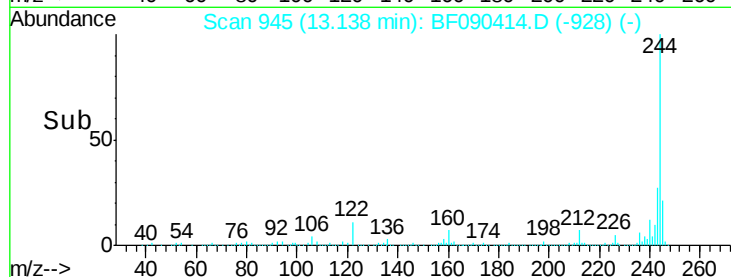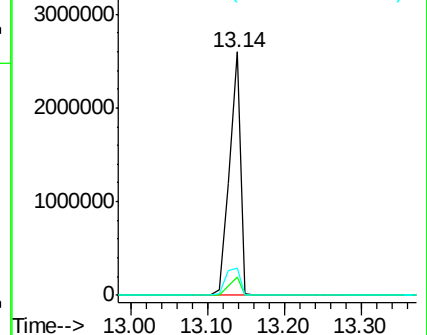

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.69 min Scan# 1168

Delta R.T. -0.01 min

Lab File: BF090414.D

Acq: 6 Oct 2016 7:06


Tgt Ion:264 Resp: 453630

Ion Ratio Lower Upper

264 100

260 24.7 19.3 28.9

265 22.0 17.4 26.0

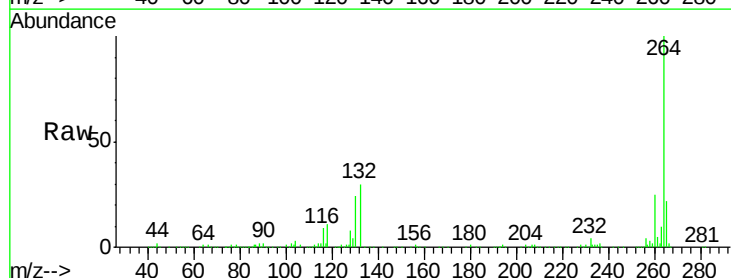

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

