


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100516\
 Data File : BF090381.D
 Acq On : 5 Oct 2016 15:08
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF100516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 05 14:57:00 2016

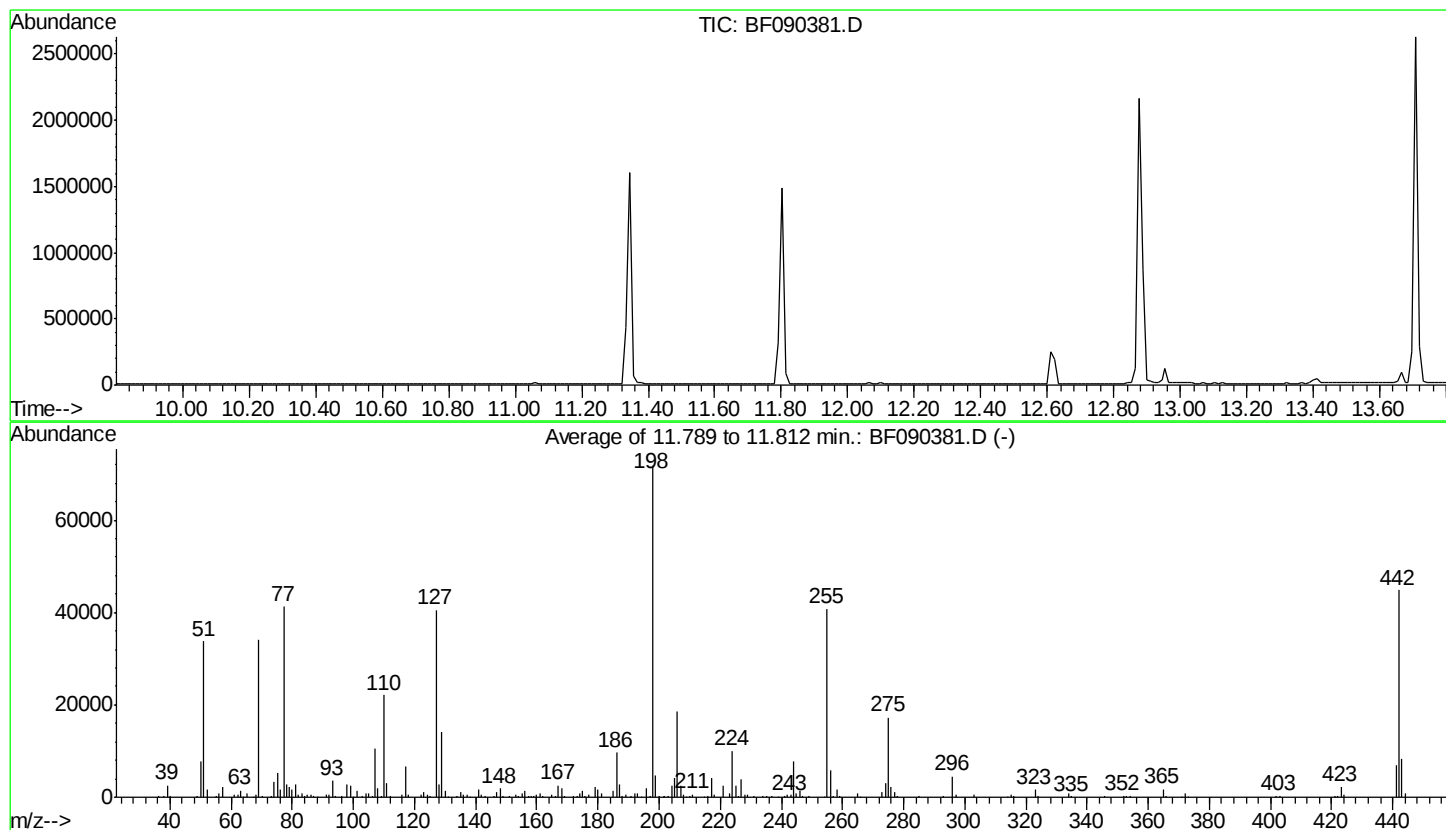

AutoFind: Scans 827, 828, 829; Background Corrected with Scan 824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.0	33740	PASS
68	69	0.00	2	1.6	535	PASS
69	198	0.00	100	47.7	34246	PASS
70	69	0.00	2	0.4	149	PASS
127	198	10	80	56.5	40549	PASS
197	198	0.00	2	0.2	168	PASS
198	198	100	100	100.0	71826	PASS
199	198	5	9	6.5	4687	PASS
275	198	10	60	24.1	17330	PASS
365	198	1	100	2.5	1779	PASS
441	442	0.01	24	15.6	6990	PASS
442	198	50	100	62.4	44805	PASS
443	442	15	24	18.7	8370	PASS