


Data Path : Z:\HPCHEM1\BNA F\DATA\BF100516\
 Data File : BF090405.D
 Acq On : 6 Oct 2016 2:57
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF100516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 05 14:57:00 2016

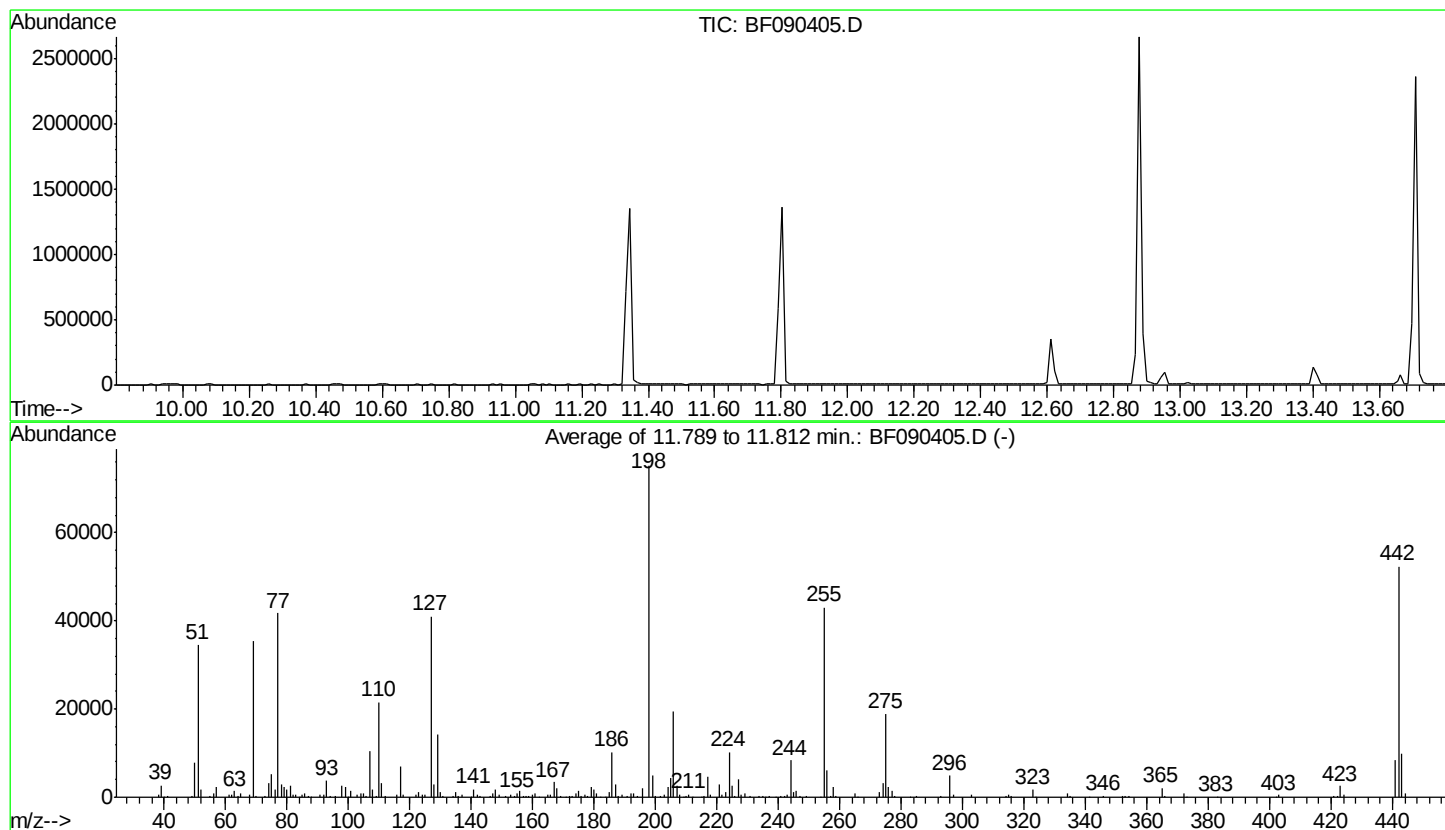

AutoFind: Scans 827, 828, 829; Background Corrected with Scan 824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	34698	PASS
68	69	0.00	2	1.4	489	PASS
69	198	0.00	100	47.0	35388	PASS
70	69	0.00	2	0.7	240	PASS
127	198	10	80	54.6	41056	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	75242	PASS
199	198	5	9	6.5	4922	PASS
275	198	10	60	25.2	18975	PASS
365	198	1	100	2.7	2051	PASS
441	442	0.01	24	16.1	8441	PASS
442	198	50	100	69.7	52432	PASS
443	442	15	24	19.0	9959	PASS