
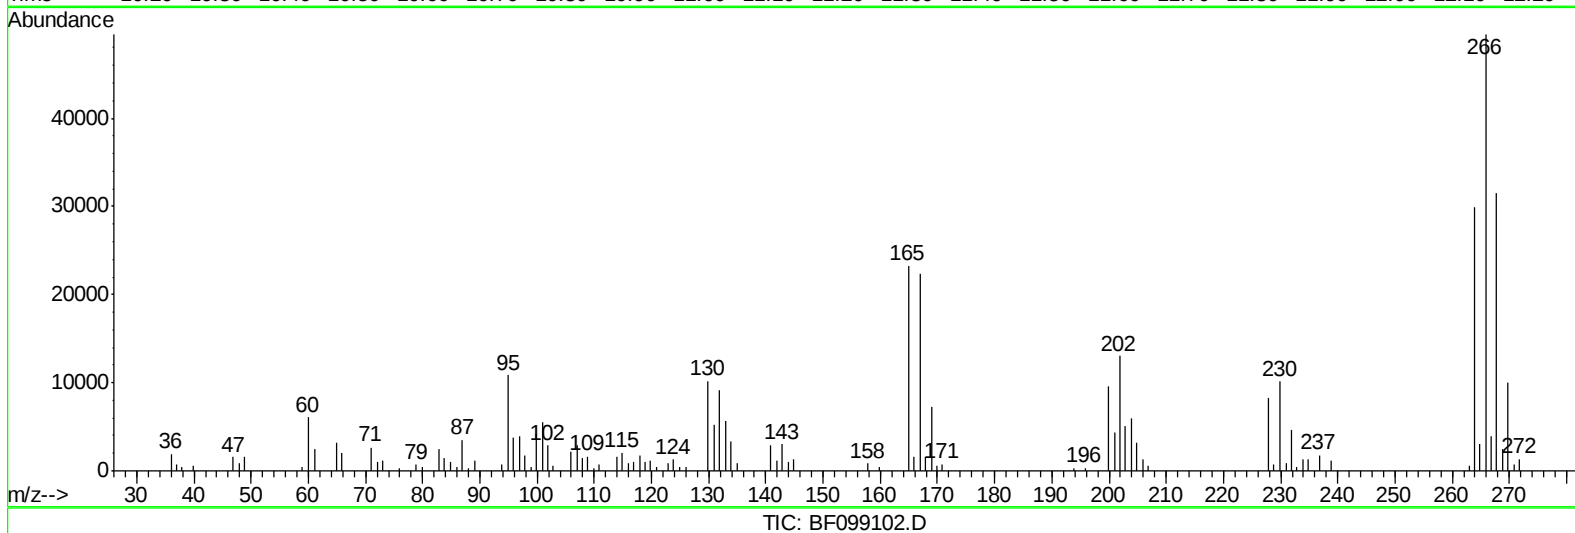


Data Path : Z:\HPCHEM1\BNA F\Data\BF100517\
Data File : BF099102.D
Acq On : 5 Oct 2017 14:40
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 01:41:21 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 05 17:20:48 2017
Response via : Initial Calibration

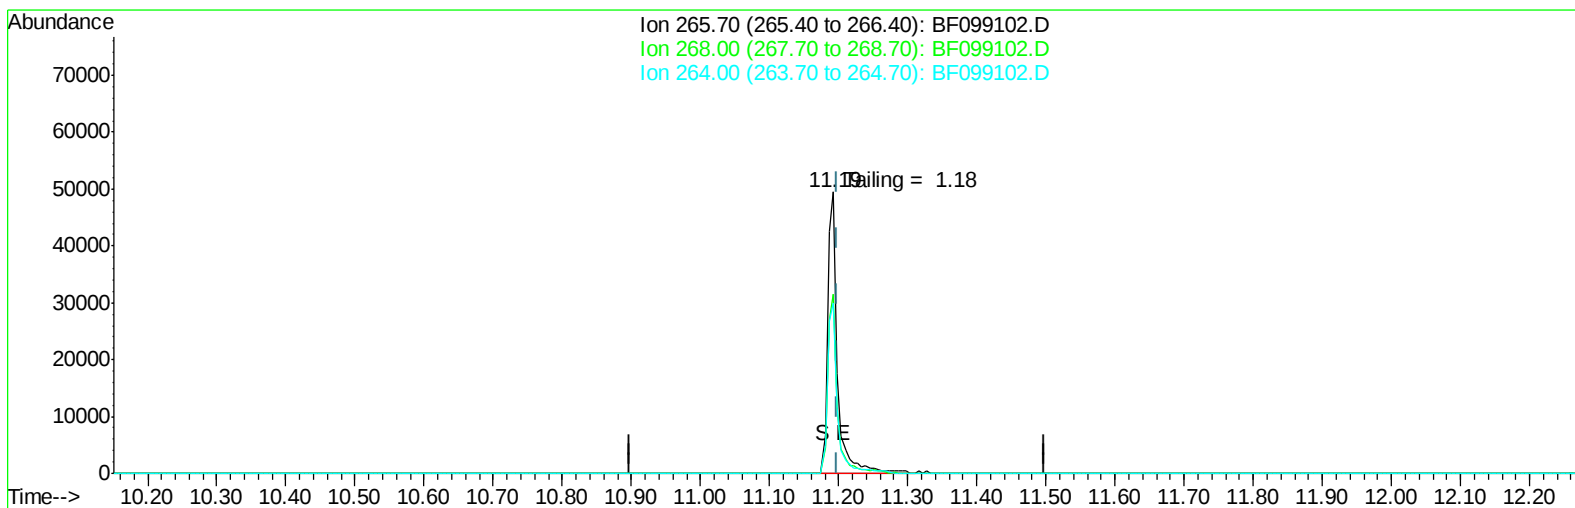

TIC: BF099102.D

(69) Pentachlorophenol (C)



11.192min (-0.006) 27364.98ng

response 49141

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.55
264.00	61.90	60.29
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF100517\
 Data File : BF099102.D
 Acq On : 5 Oct 2017 14:40
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 01:41:21 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 05 17:20:48 2017
 Response via : Initial Calibration

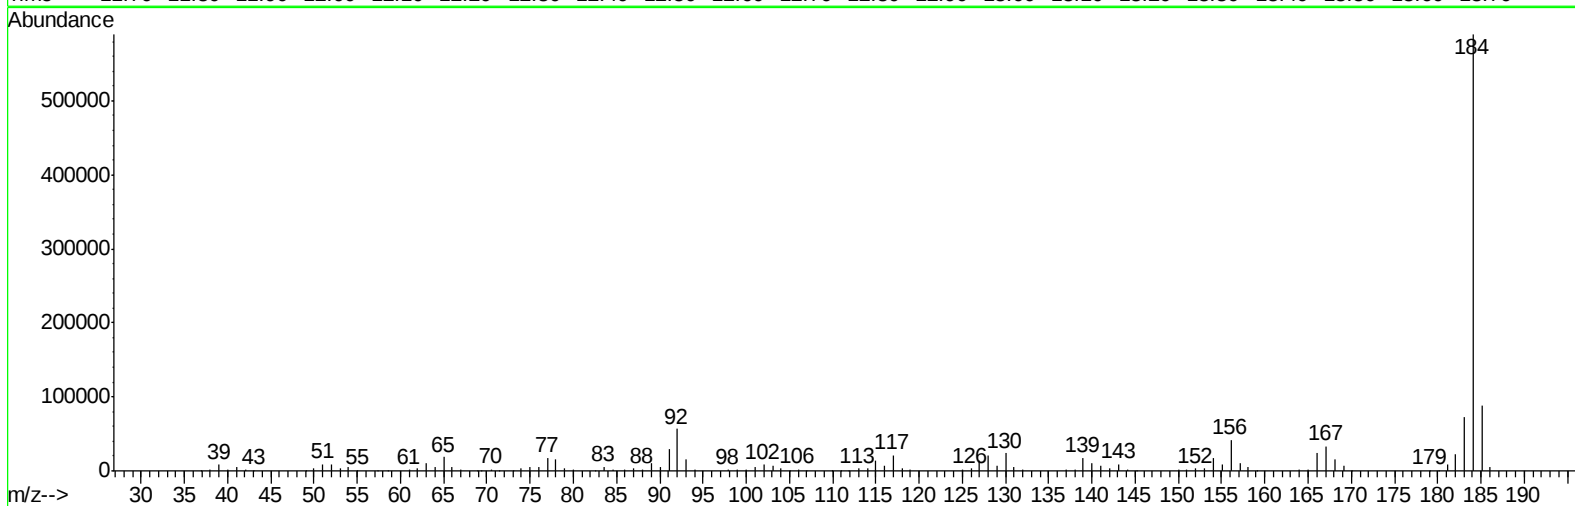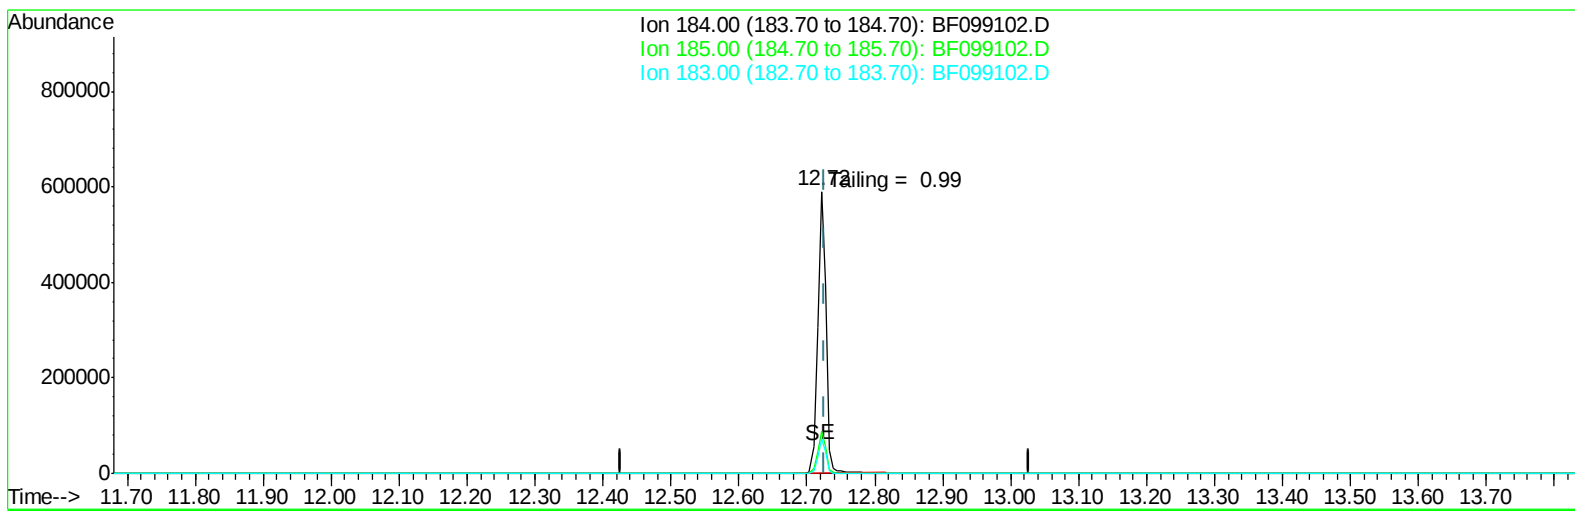

TIC: BF099102.D

(76) Benzidine

12.721min (-0.006) 0.00ng

response 509650

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.09
183.00	11.60	12.19
0.00	0.00	0.00