
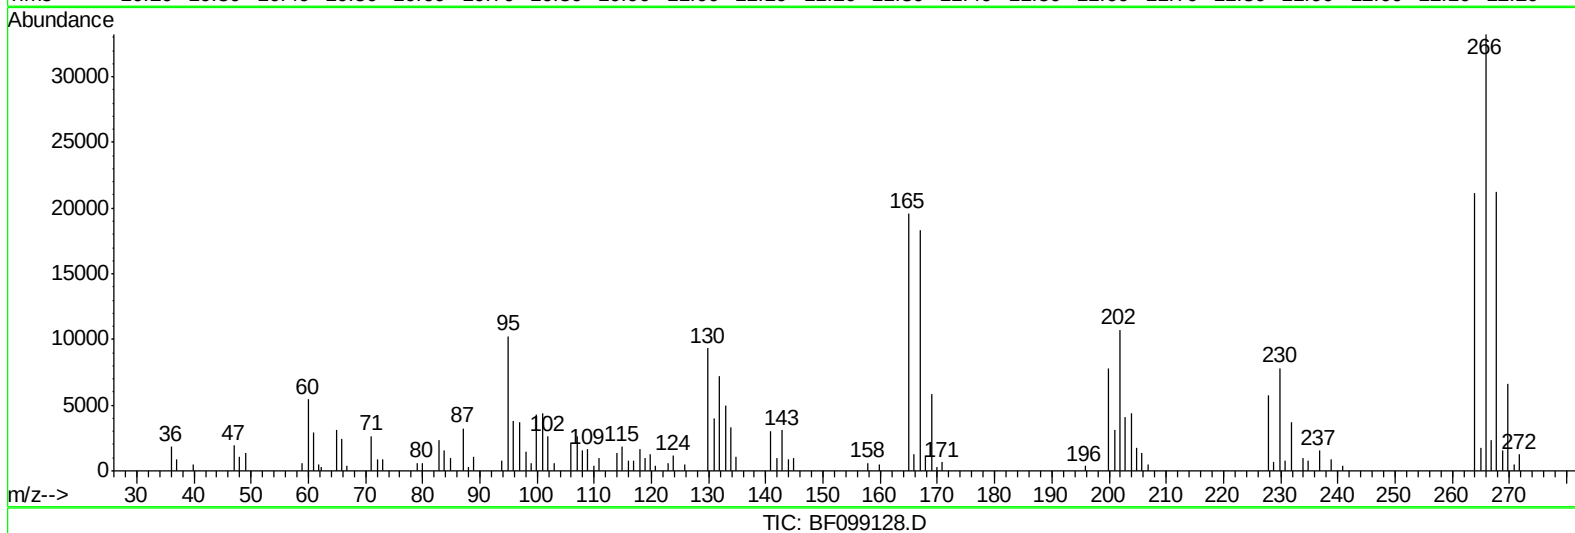


Data Path : Z:\HPCHEM1\BNA F\Data\BF100517\
Data File : BF099128.D
Acq On : 6 Oct 2017 4:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 08:05:02 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 05 17:20:48 2017
Response via : Initial Calibration

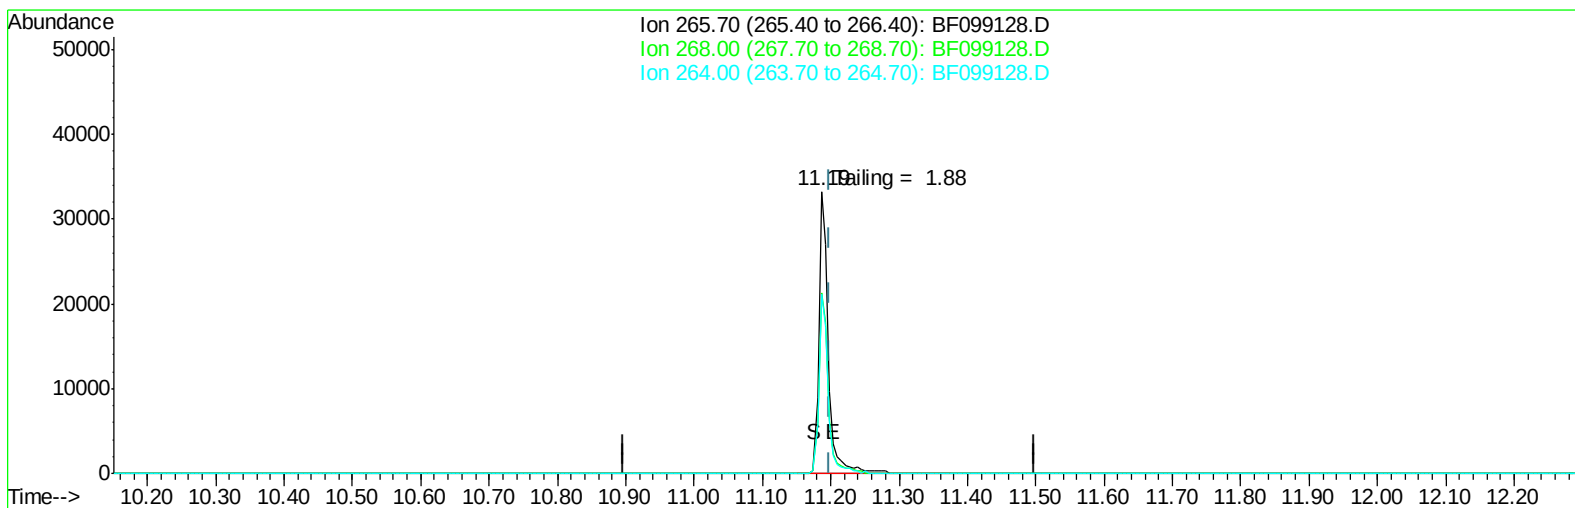

TIC: BF099128.D

(69) Pentachlorophenol (C)



11.186min (-0.012) 35209.28ng

response 32301

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.95
264.00	61.90	63.56
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF100517\
Data File : BF099128.D
Acq On : 6 Oct 2017 4:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 08:05:02 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 05 17:20:48 2017
Response via : Initial Calibration

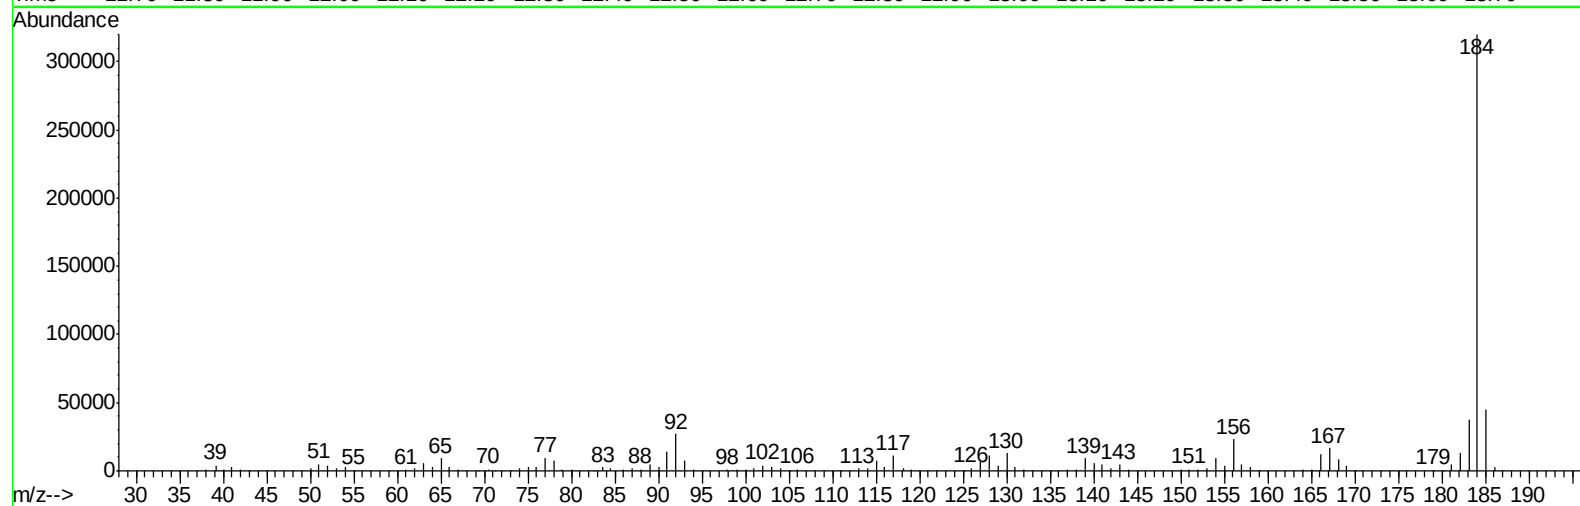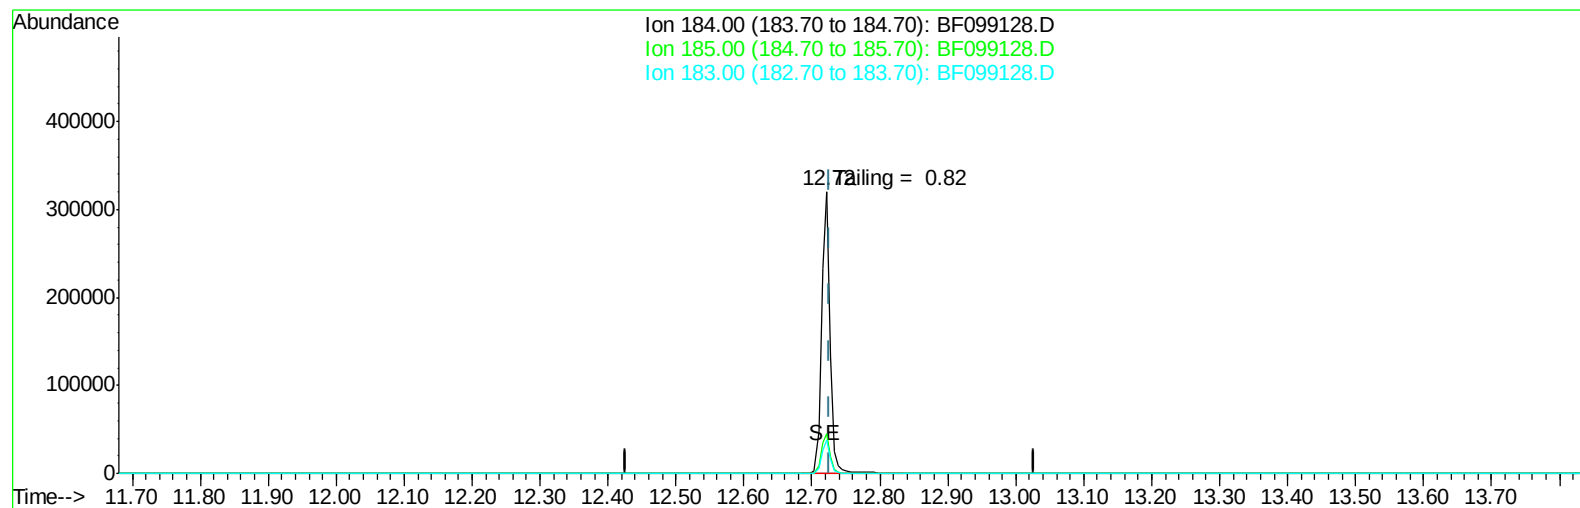

TIC: BF099128.D

(76) Benzidine

12.721min (-0.006) 0.00ng

response 279345

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.19
183.00	11.60	11.61
0.00	0.00	0.00