

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100517\
 Data File : BF099126.D
 Acq On : 6 Oct 2017 1:53
 Operator : SJ/JU
 Sample : I5585-19 20X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G71-1.5-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.081	506	509	519	rVB	9059	9992	1.23%	0.220%
2	5.475	572	576	584	rBV	72297	67285	8.25%	1.481%
3	6.481	744	747	753	rBV	71408	66952	8.21%	1.473%
4	6.628	769	772	776	rBV	95585	74449	9.13%	1.638%
5	6.863	808	812	815	rBV	793188	622703	76.35%	13.704%
6	7.016	835	838	842	rVB	71309	57242	7.02%	1.260%
7	7.422	904	907	913	rVB	51190	41110	5.04%	0.905%
8	8.145	1026	1030	1033	rBV	1013535	815578	100.00%	17.948%
9	9.216	1209	1212	1220	rVB	101380	75982	9.32%	1.672%
10	9.898	1324	1328	1332	rBV2	910066	759299	93.10%	16.710%
11	10.686	1459	1462	1465	rBV	17821	14723	1.81%	0.324%
12	11.386	1577	1581	1584	rBV	691211	594095	72.84%	13.074%
13	12.827	1823	1826	1827	rBV	10270	10019	1.23%	0.220%
14	12.845	1827	1829	1837	rVB	34200	39099	4.79%	0.860%
15	12.963	1846	1849	1853	rVB	64844	47311	5.80%	1.041%
16	14.021	2025	2029	2033	rBV	652931	602487	73.87%	13.259%
17	14.280	2071	2073	2075	rBV3	11883	13679	1.68%	0.301%
18	15.498	2275	2280	2289	rVB	495829	632093	77.50%	13.910%


Sum of corrected areas: 4544098

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100517\
Data File : BF099126.D
Acq On : 6 Oct 2017 1:53
Operator : SJ/JU
Sample : I5585-19 20X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G71-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

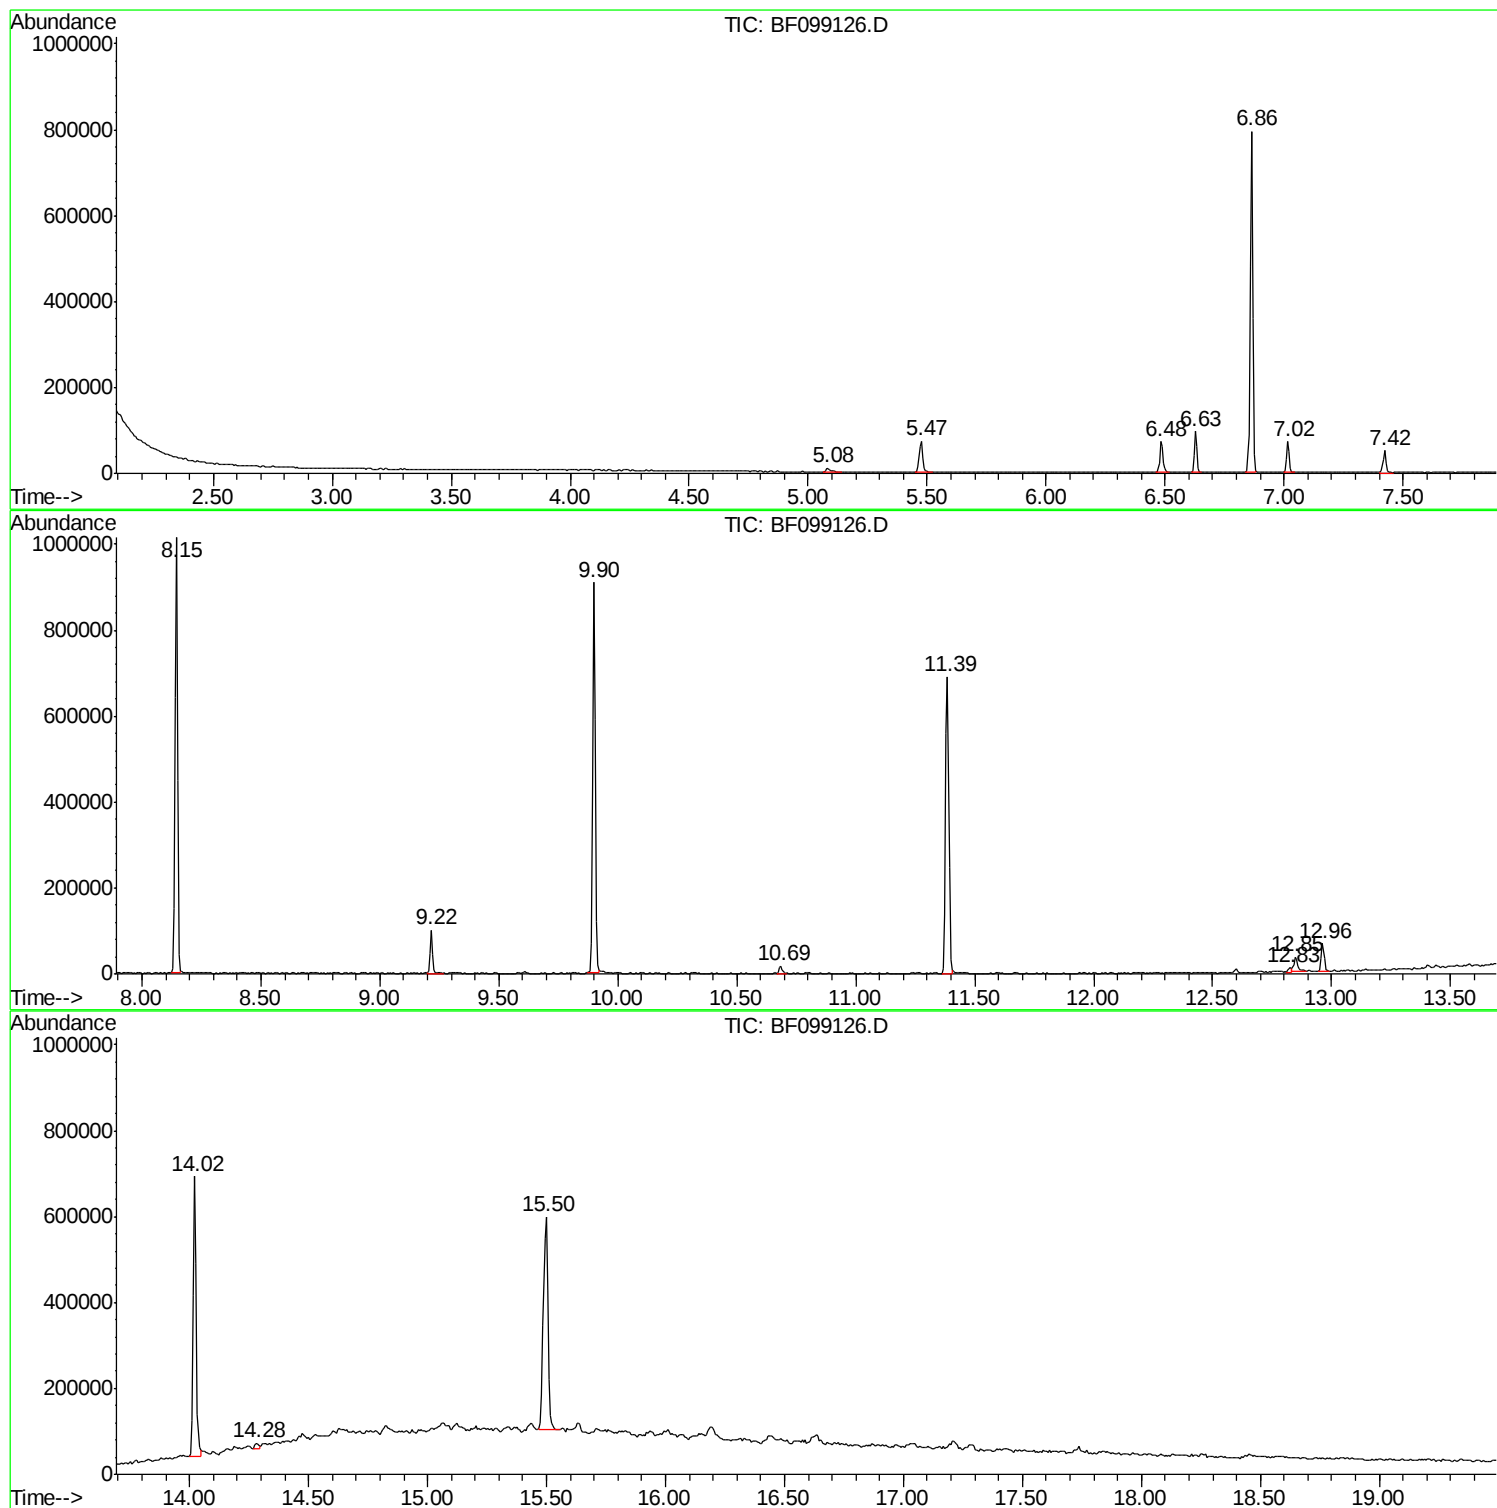

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100517\
Data File : BF099126.D
Acq On : 6 Oct 2017 1:53
Operator : SJ/JU
Sample : I5585-19 20X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G71-1.5-3










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.63 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.63	2.39 ng	74449	1,4-Dichlorobenzene-d4	6.86

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	30
2			5-Aminoindole	132	C8H8N2	005192-03-0	10
3			2H-Cyclopenta[d]pyridazine, 2-methyl-	132	C8H8N2	022291-85-6	9
4			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5			Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	9

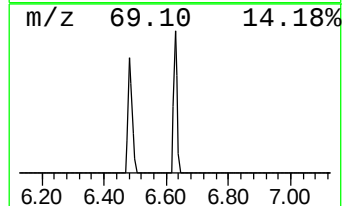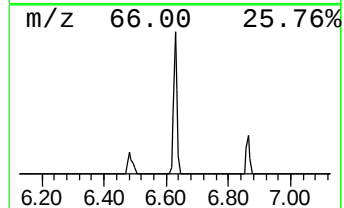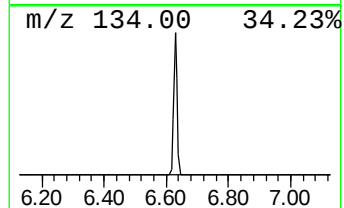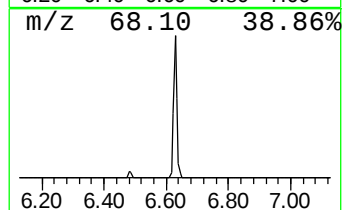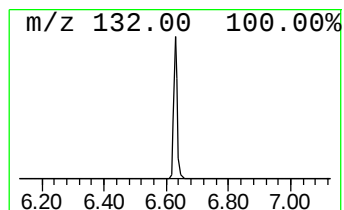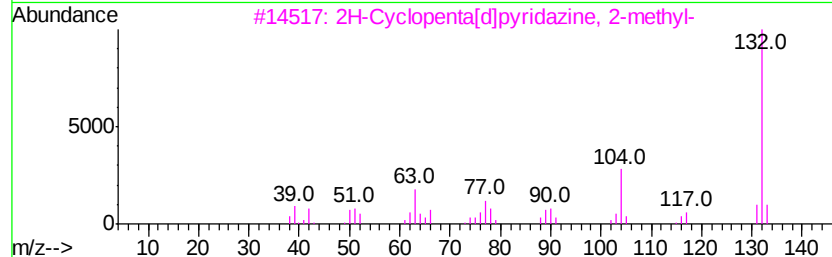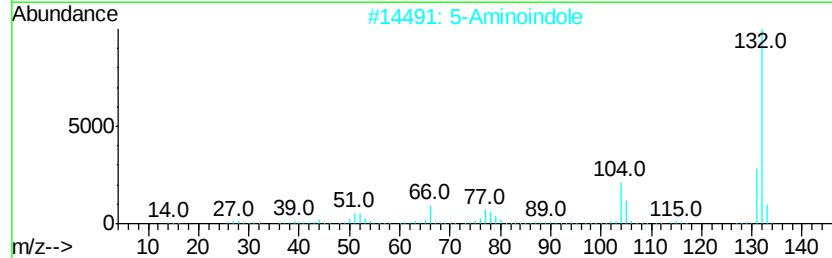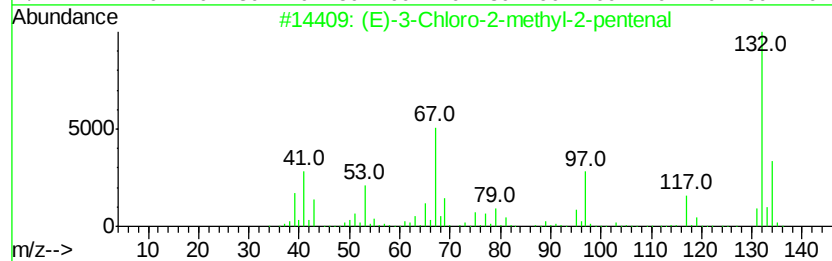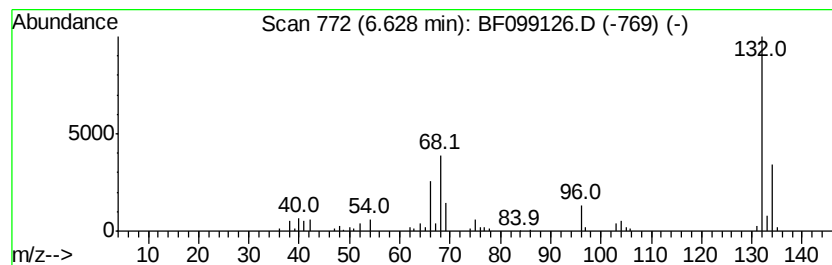

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100517\
Data File : BF099126.D
Acq On : 6 Oct 2017 1:53
Operator : SJ/JU
Sample : I5585-19 20X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G71-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.63	6.63	2.4	ng	74449	1	6.86	622703	20.0