


Data Path : Z:\HPCHEM1\BNA F\DATA\BF100517\
Data File : BF099102.D
Acq On : 5 Oct 2017 14:40
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 05 17:20:48 2017

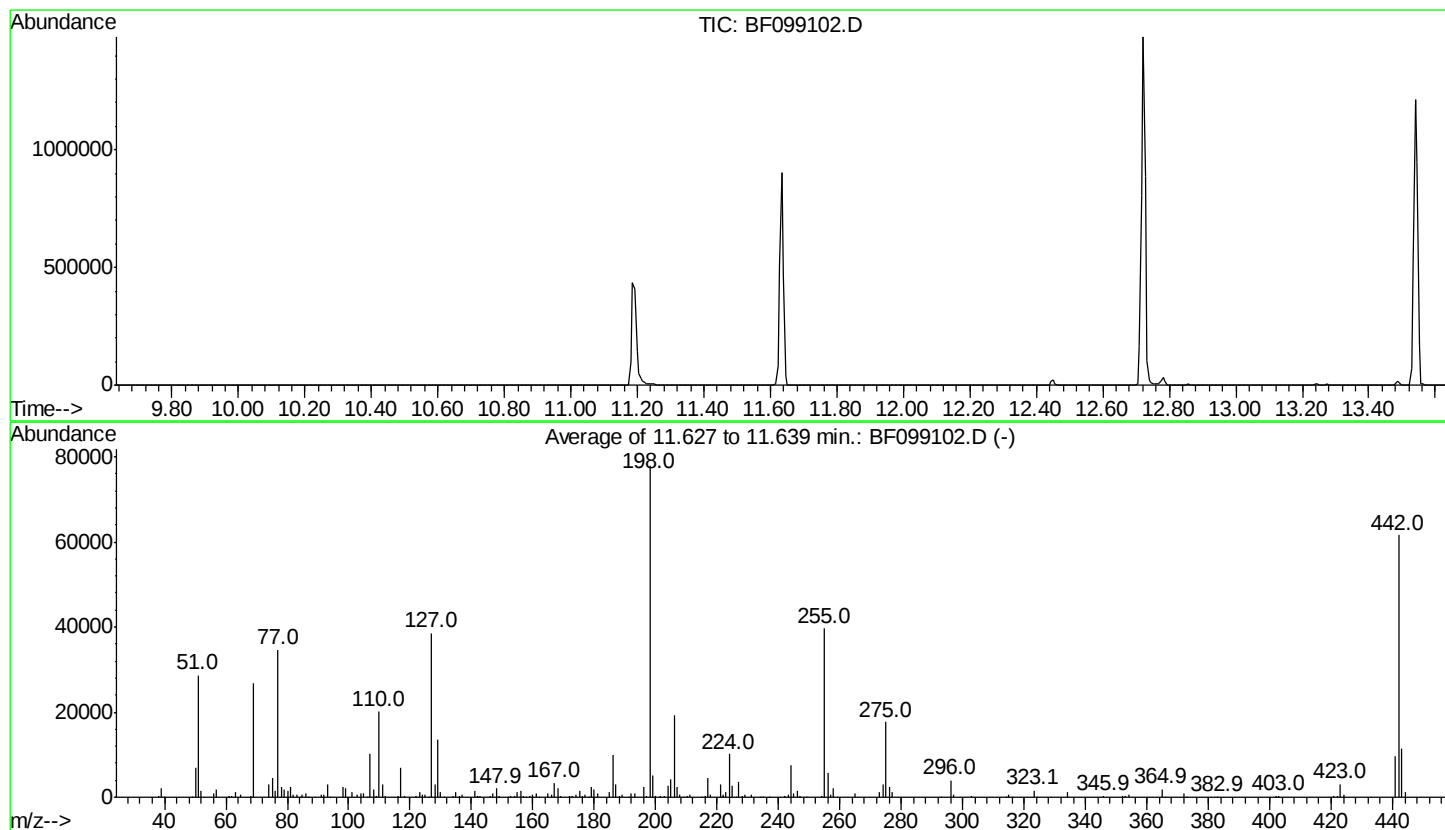

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	28588	PASS
68	69	0.00	2	1.5	415	PASS
69	198	0.00	100	34.5	26874	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.4	38525	PASS
197	198	0.00	2	0.6	437	PASS
198	198	100	100	100.0	77914	PASS
199	198	5	9	6.4	4977	PASS
275	198	10	60	22.8	17740	PASS
365	198	1	100	2.3	1827	PASS
441	442	0.01	24	15.5	9562	PASS
442	198	50	100	79.0	61560	PASS
443	442	15	24	18.5	11363	PASS