
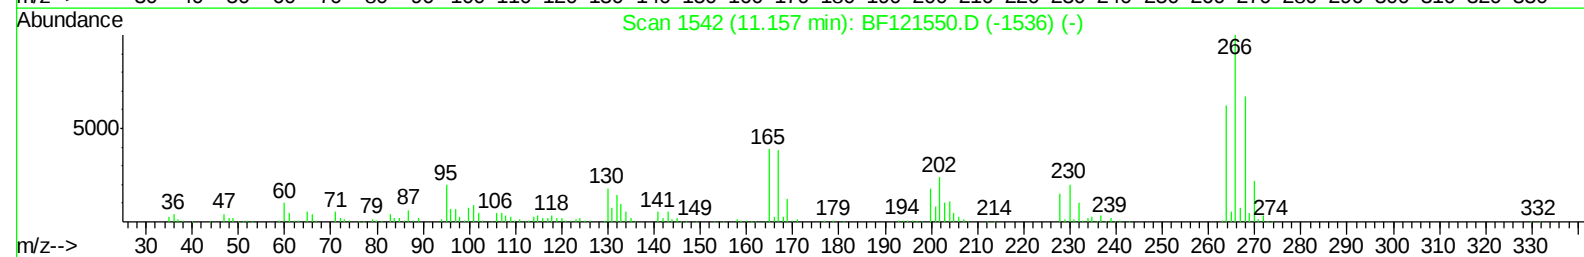
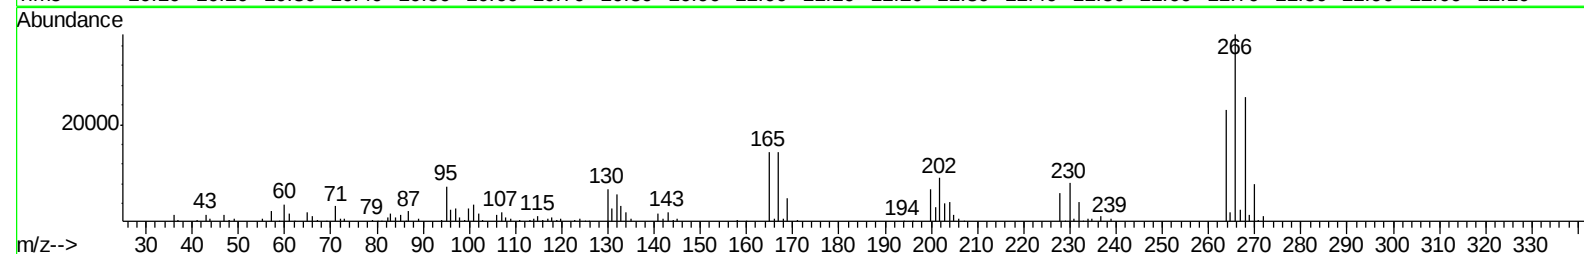


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100520\
 Data File : BF121809.D
 Acq On : 5 Oct 2020 9:22
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 08:12:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 01 14:29:14 2020
 Response via : Initial Calibration

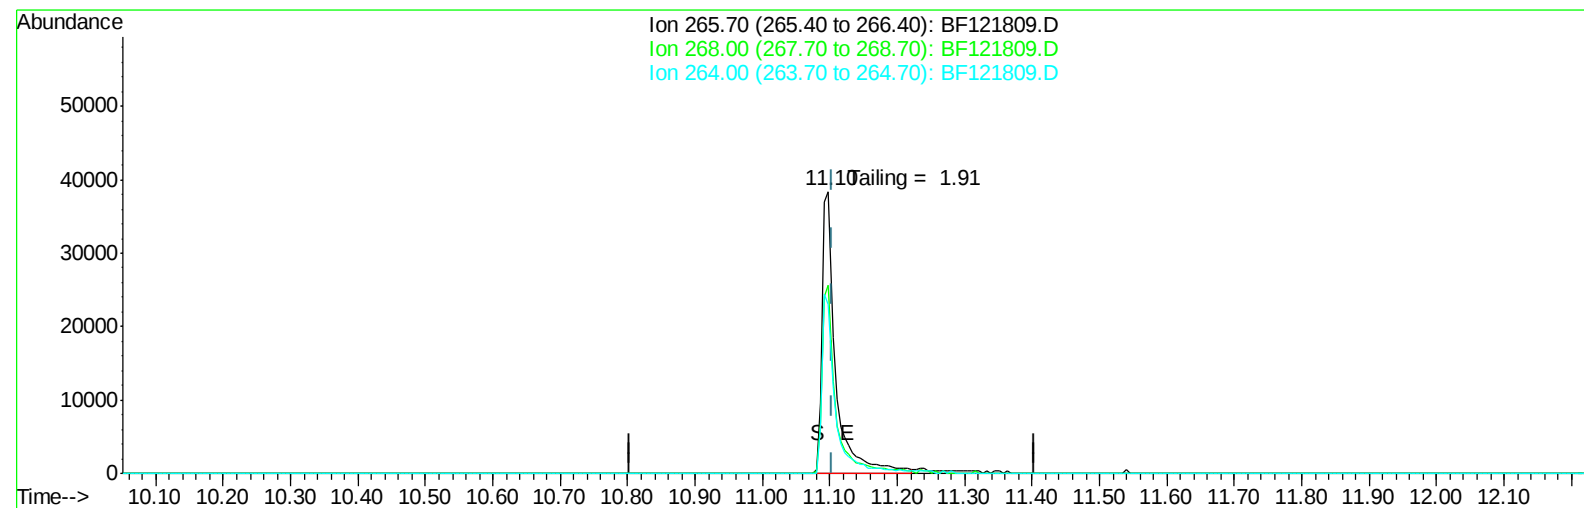

TIC: BF121809.D

(70) Pentachlorophenol (C)




11.098min (-0.006) 26444.49ng

response 52622

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	66.95
264.00	62.40	60.05
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100520\
 Data File : BF121809.D
 Acq On : 5 Oct 2020 9:22
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 08:12:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 01 14:29:14 2020
 Response via : Initial Calibration

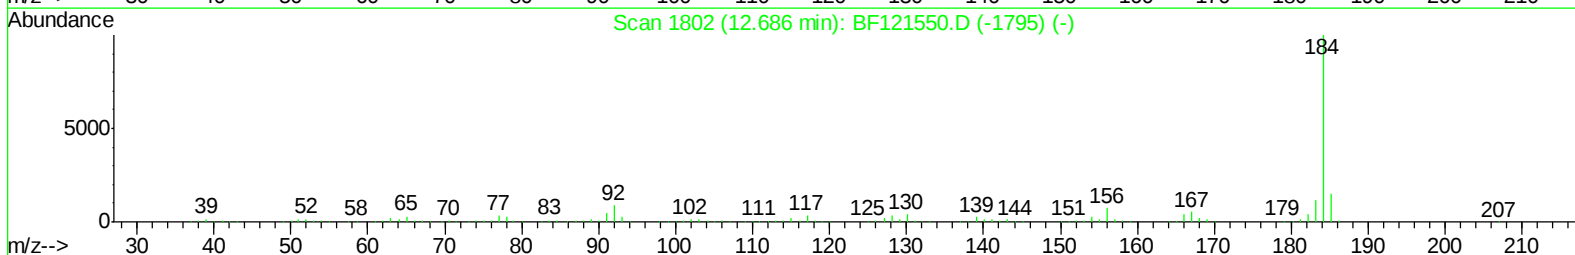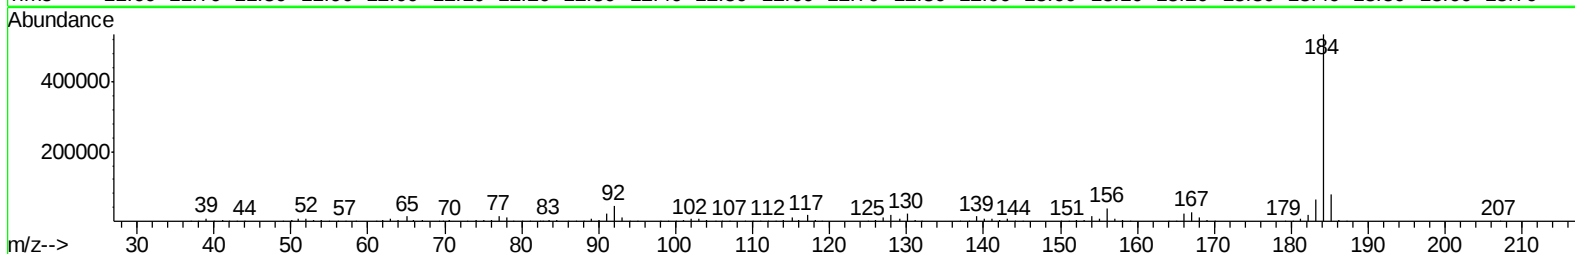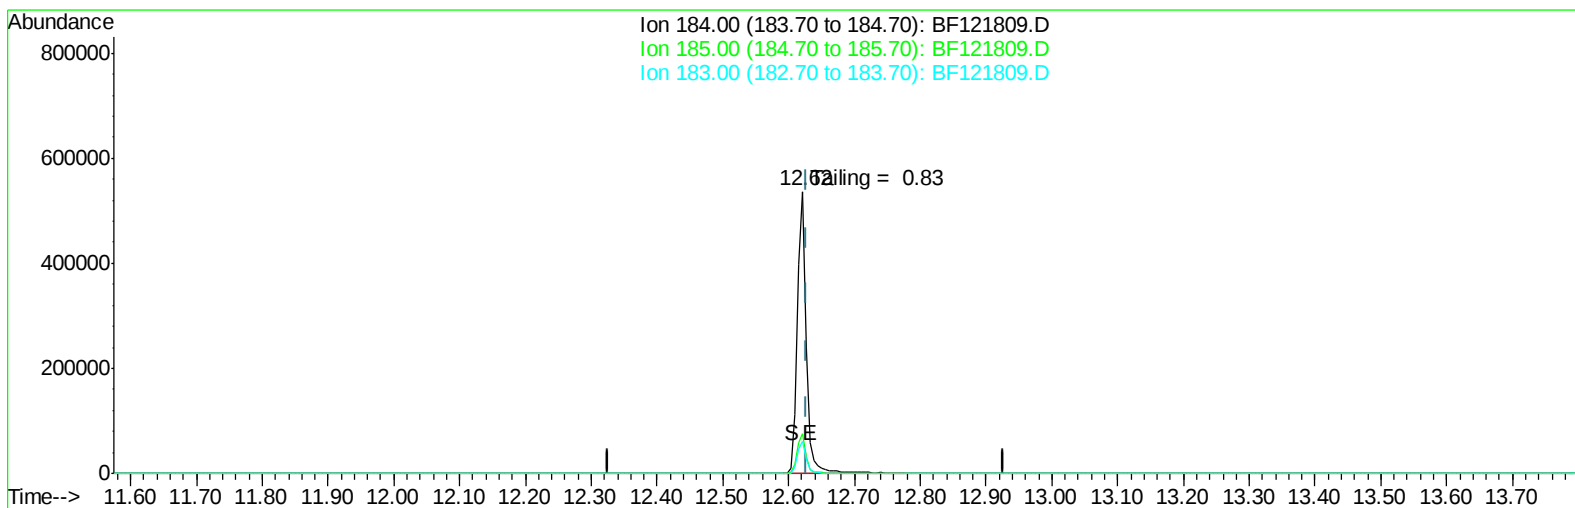

TIC: BF121809.D

(77) Benzidine

12.621min (-0.006) 0.00ng

response 512528

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	14.17
183.00	11.70	11.59
0.00	0.00	0.00