
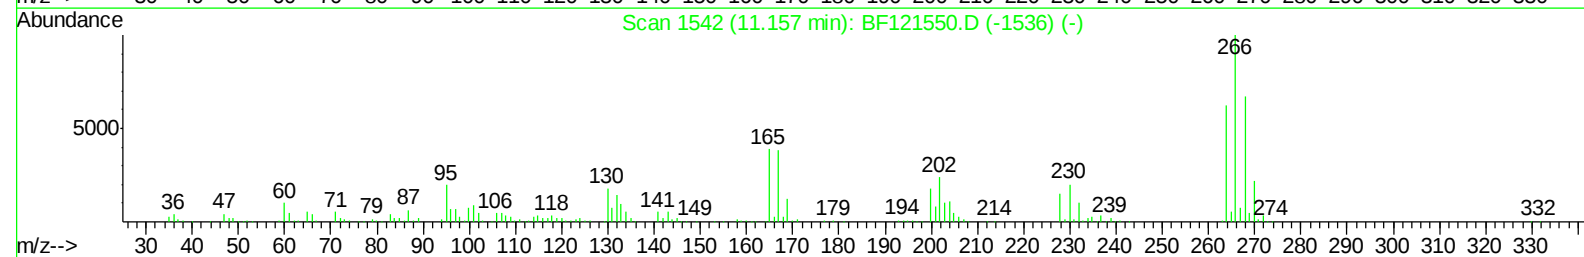
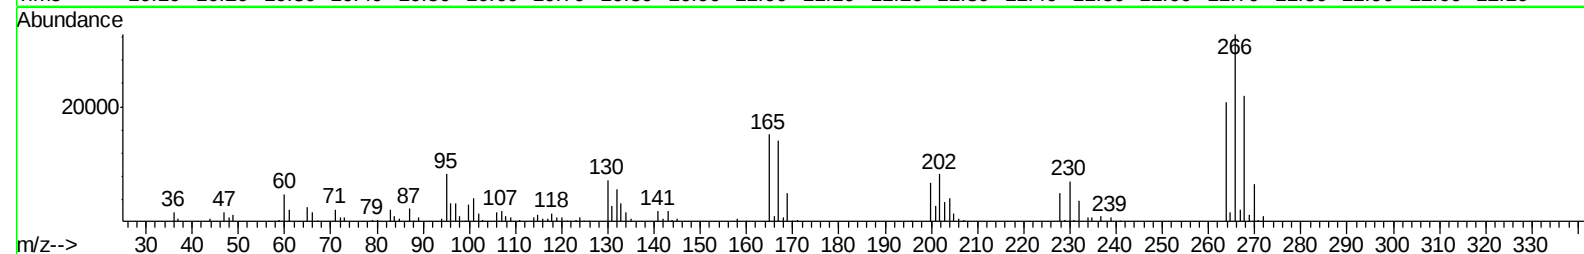


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF100520\
 Data File : BF121818.D
 Acq On : 5 Oct 2020 15:06
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 00:10:58 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 01 14:29:14 2020
 Response via : Initial Calibration

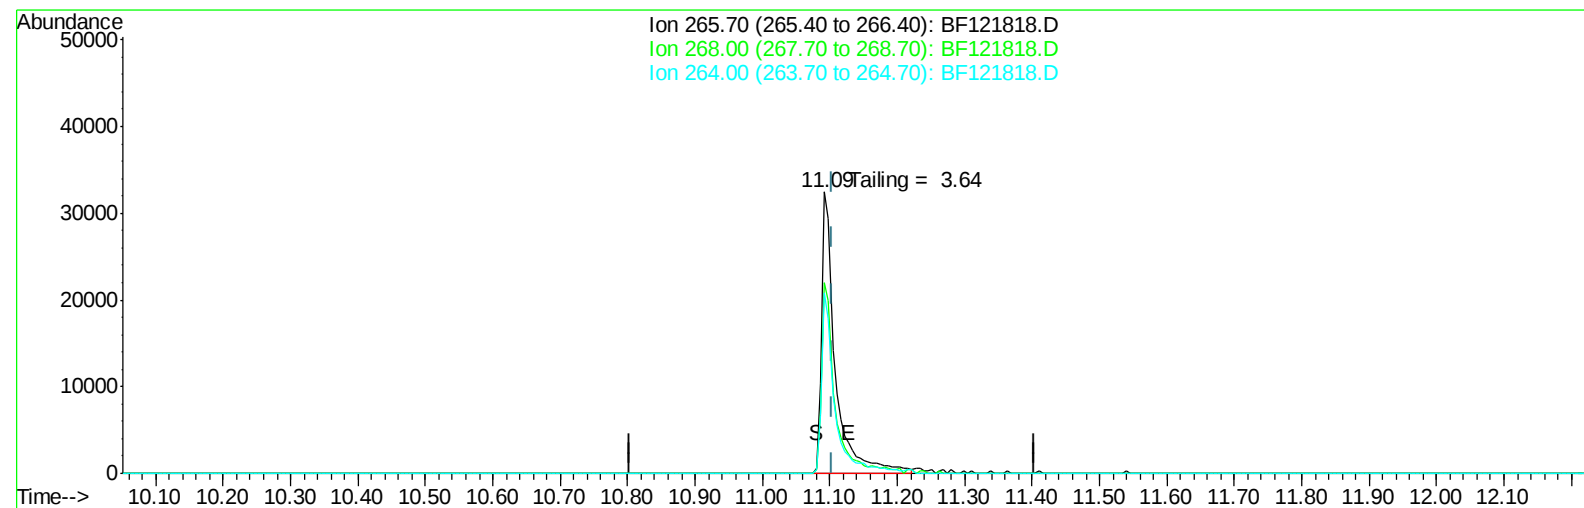

TIC: BF121818.D

(70) Pentachlorophenol (C)




11.092min (-0.012) 48243.95ng

response 45277

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	67.78
264.00	62.40	63.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF100520\
Data File : BF121818.D
Acq On : 5 Oct 2020 15:06
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 00:10:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 01 14:29:14 2020
Response via : Initial Calibration

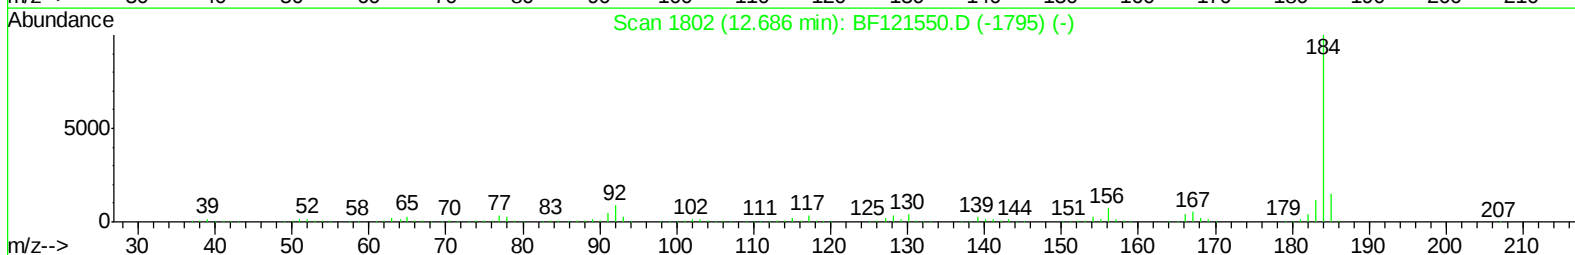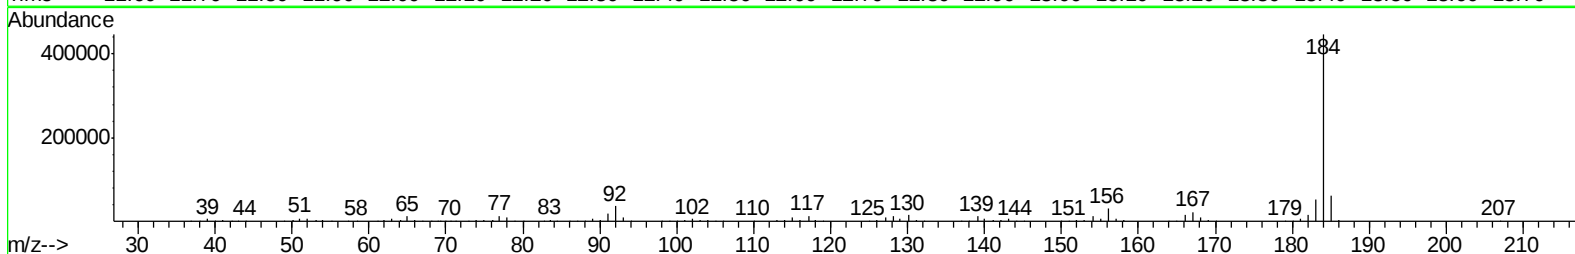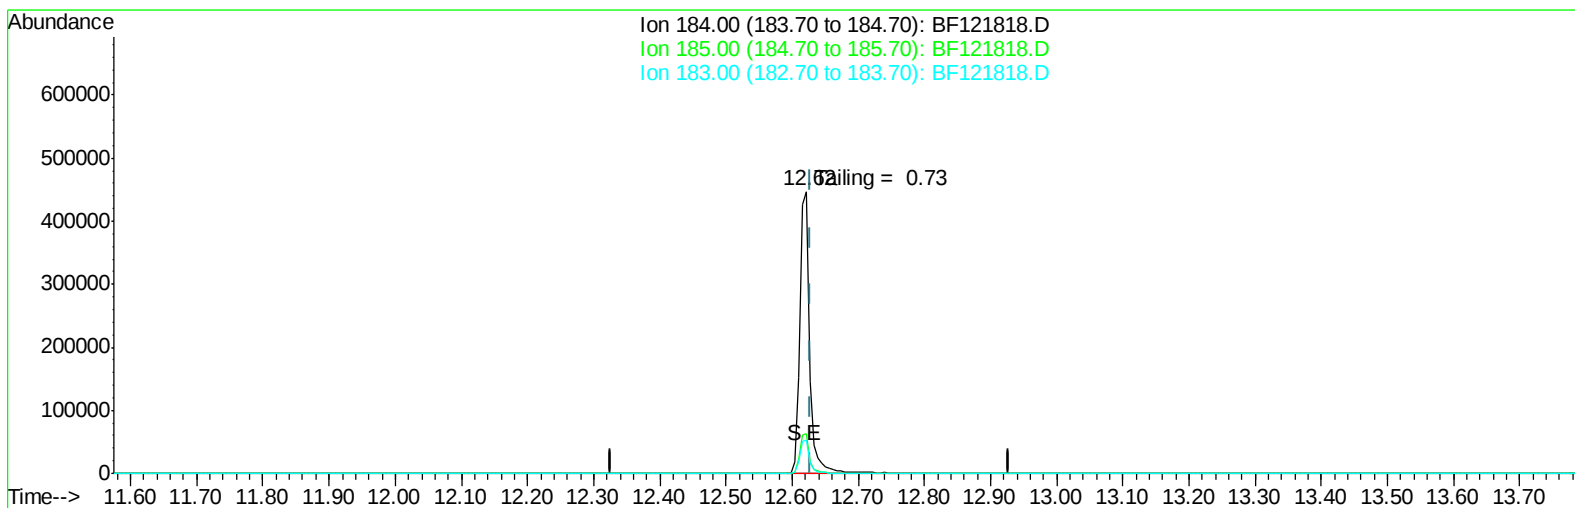

TIC: BF121818.D

(77) Benzidine

12.622min (-0.006) 0.00ng

response 471019

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	13.90
183.00	11.70	11.69
0.00	0.00	0.00