

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100520\
Data File : BF121820.D
Acq On : 5 Oct 2020 16:40
Operator : JU/CG
Sample : PB132087BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132087BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.987	490	493	505	rVB	36482	54328	1.13%	0.209%
2	5.387	557	561	580	rBV	3077389	3130118	65.39%	12.028%
3	6.404	729	734	737	rBV	2928807	3073242	64.20%	11.809%
4	6.763	791	795	798	rBV	817362	701271	14.65%	2.695%
5	7.328	886	891	894	rBV	2193560	2186439	45.67%	8.401%
6	8.045	1008	1013	1028	rBV	1007511	936918	19.57%	3.600%
7	9.122	1190	1196	1199	rBV	3845667	3896327	81.39%	14.972%
8	9.798	1306	1311	1320	rBV	1212625	1113318	23.26%	4.278%
9	10.586	1441	1445	1463	rBV	2430725	2542944	53.12%	9.771%
10	11.280	1559	1563	1571	rBV	1300012	1208419	25.24%	4.643%
11	12.874	1828	1834	1837	rBV	4461079	4786990	100.00%	18.394%
12	13.921	2007	2012	2019	rBV	1208561	1214757	25.38%	4.668%
13	15.356	2250	2256	2267	rVB	909243	1179601	24.64%	4.533%


Sum of corrected areas: 26024672

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100520\
Data File : BF121820.D
Acq On : 5 Oct 2020 16:40
Operator : JU/CG
Sample : PB132087BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132087BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

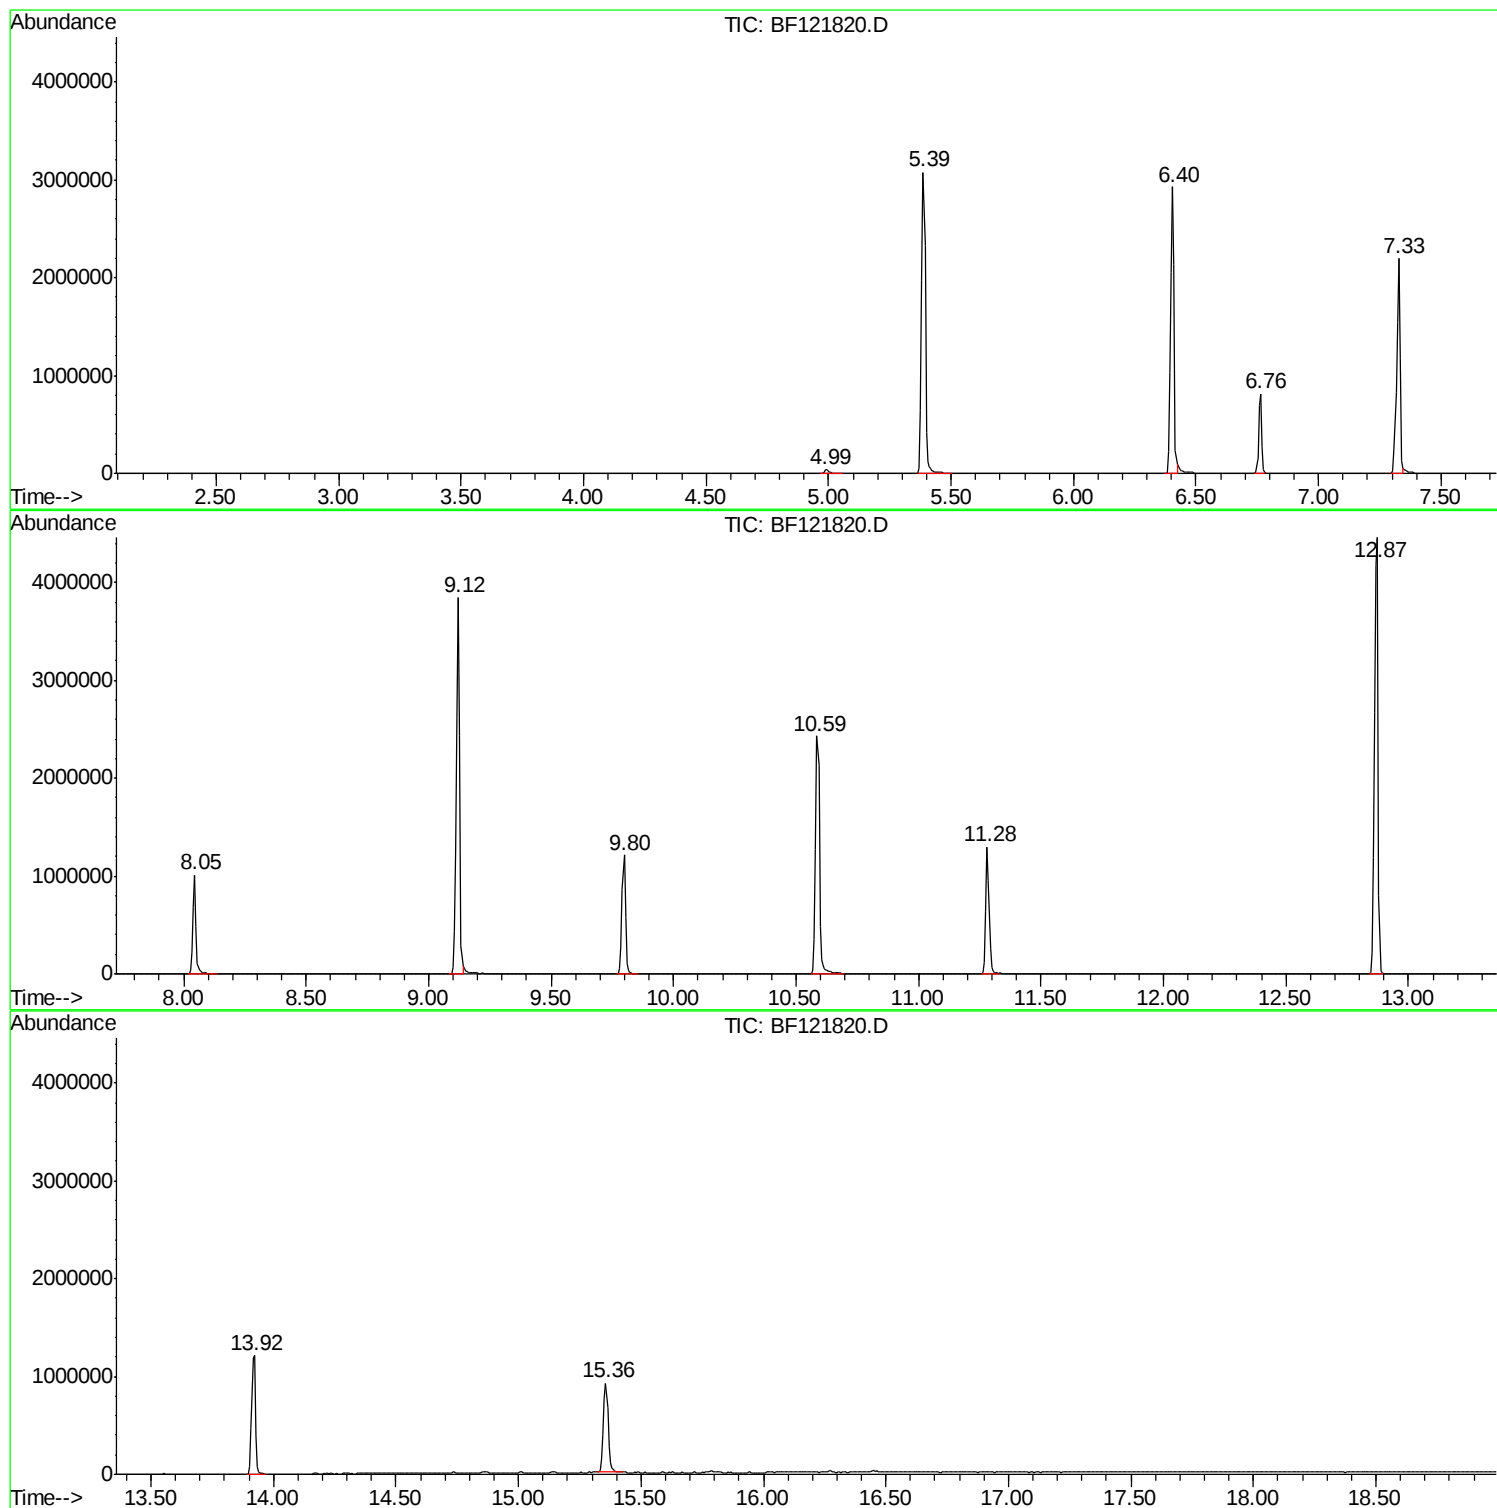

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF100520\
Data File : BF121820.D
Acq On : 5 Oct 2020 16:40
Operator : JU/CG
Sample : PB132087BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132087BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF100520\
Data File : BF121820.D
Acq On : 5 Oct 2020 16:40
Operator : JU/CG
Sample : PB132087BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132087BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc