


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100520\
 Data File : BF121809.D
 Acq On : 5 Oct 2020 9:22
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 01 14:29:14 2020

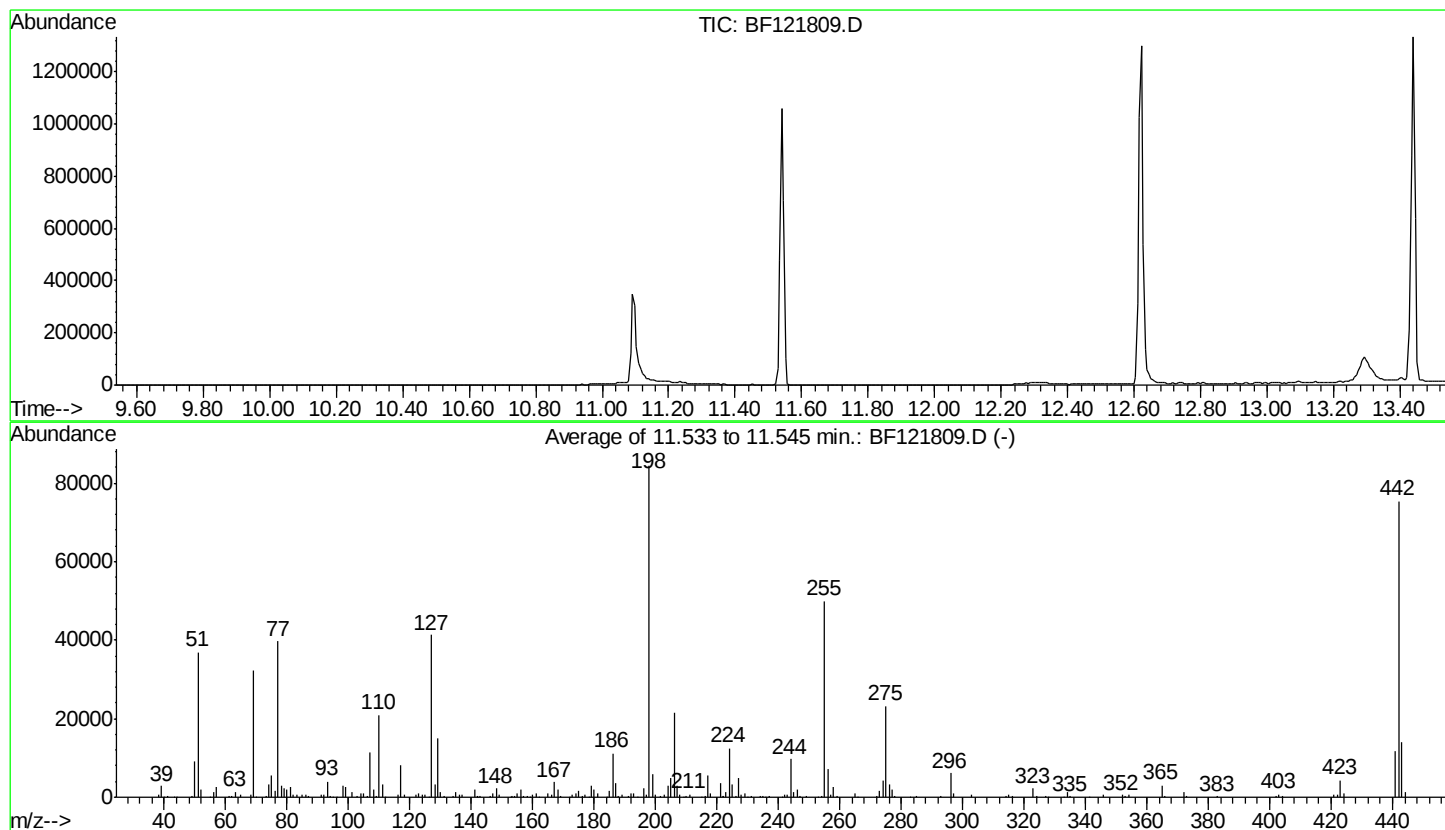

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.8	36989	PASS
68	69	0.00	2	1.8	586	PASS
69	198	0.00	100	38.2	32277	PASS
70	69	0.00	2	0.3	102	PASS
127	198	10	80	49.0	41378	PASS
197	198	0.00	2	0.6	506	PASS
198	198	100	100	100.0	84472	PASS
199	198	5	9	6.9	5816	PASS
275	198	10	60	27.5	23251	PASS
365	198	1	100	3.5	2959	PASS
441	198	0.01	100	13.9	11761	PASS
442	198	50	100	89.2	75354	PASS
443	442	15	24	18.7	14083	PASS