


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF100520\
 Data File : BF121818.D
 Acq On : 5 Oct 2020 15:06
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 01 14:29:14 2020

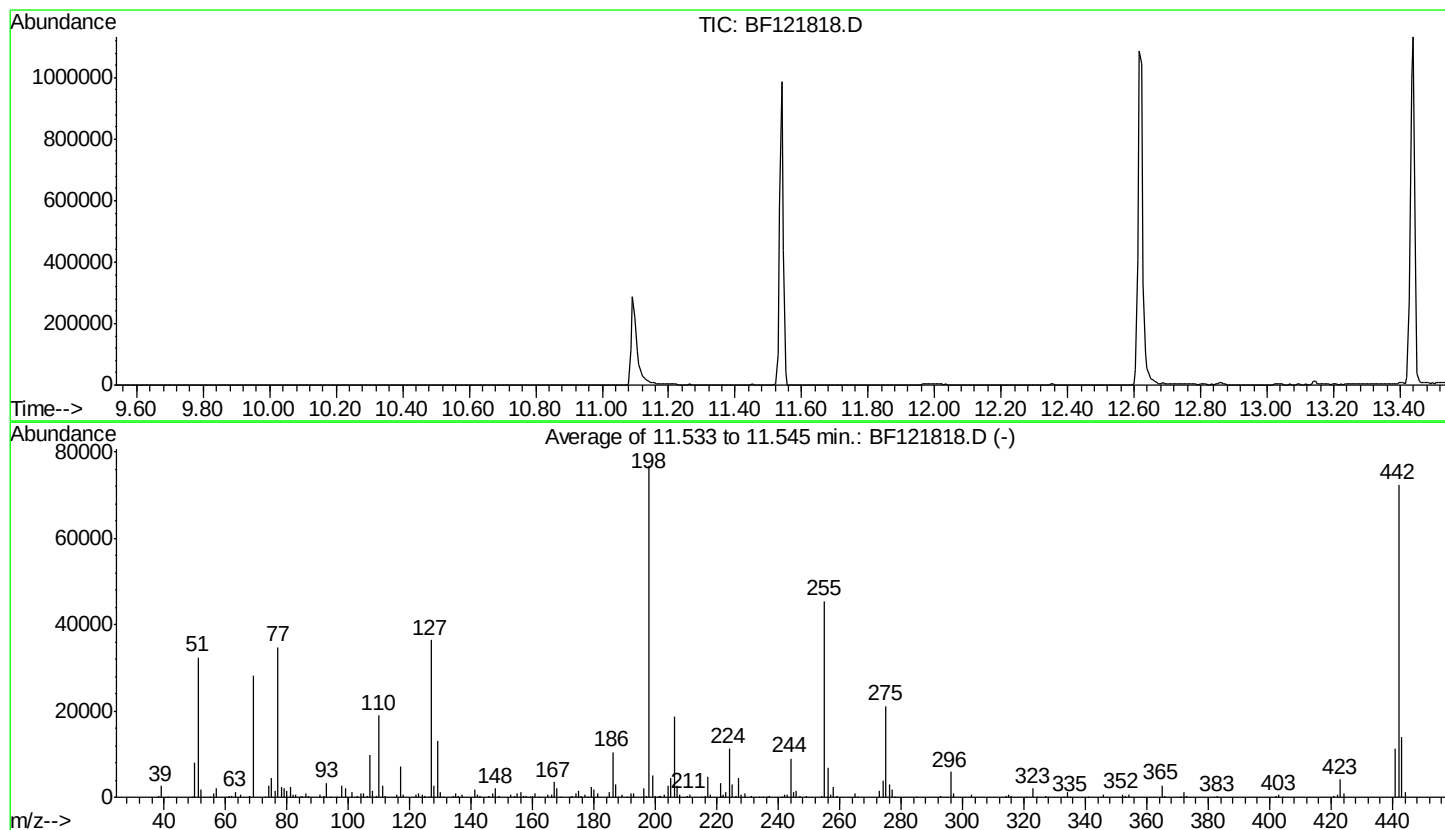

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	32326	PASS
68	69	0.00	2	1.5	429	PASS
69	198	0.00	100	36.5	28068	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.3	36362	PASS
197	198	0.00	2	0.3	251	PASS
198	198	100	100	100.0	76797	PASS
199	198	5	9	6.7	5166	PASS
275	198	10	60	27.6	21163	PASS
365	198	1	100	3.7	2826	PASS
441	198	0.01	100	14.6	11221	PASS
442	198	50	100	94.3	72410	PASS
443	442	15	24	19.1	13800	PASS