

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100615\
 Data File : BF082078.D
 Acq On : 6 Oct 2015 12:04
 Operator : UM/IZ
 Sample : PB85739BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB85739BL

Quant Time: Oct 07 02:17:47 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 07 02:00:35 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.88	152	80847	20.00	ng	0.00
21) Naphthalene-d8	8.17	136	309301	20.00	ng	0.00
38) Acenaphthene-d10	9.92	164	146428	20.00	ng	-0.01
63) Phenanthrene-d10	11.42	188	307012	20.00	ng	0.00
75) Chrysene-d12	14.06	240	316470	20.00	ng	-0.01
86) Perylene-d12	15.51	264	264689	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.49	112	508972	114.28	ng	0.01
7) Phenol-d6	6.51	99	634231	113.17	ng	0.00
23) Nitrobenzene-d5	7.45	82	418112	90.11	ng	0.00
41) 2,4,6-Tribromophenol	10.72	330	198355	133.76	ng	0.00
44) 2-Fluorobiphenyl	9.25	172	791628	91.91	ng	0.00
78) Terphenyl-d14	13.01	244	955100	103.66	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100615\
Data File : BF082078.D
Acq On : 6 Oct 2015 12:04
Operator : UM/IZ
Sample : PB85739BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB85739BL

Quant Time: Oct 07 02:17:47 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 07 02:00:35 2015
Response via : Initial Calibration

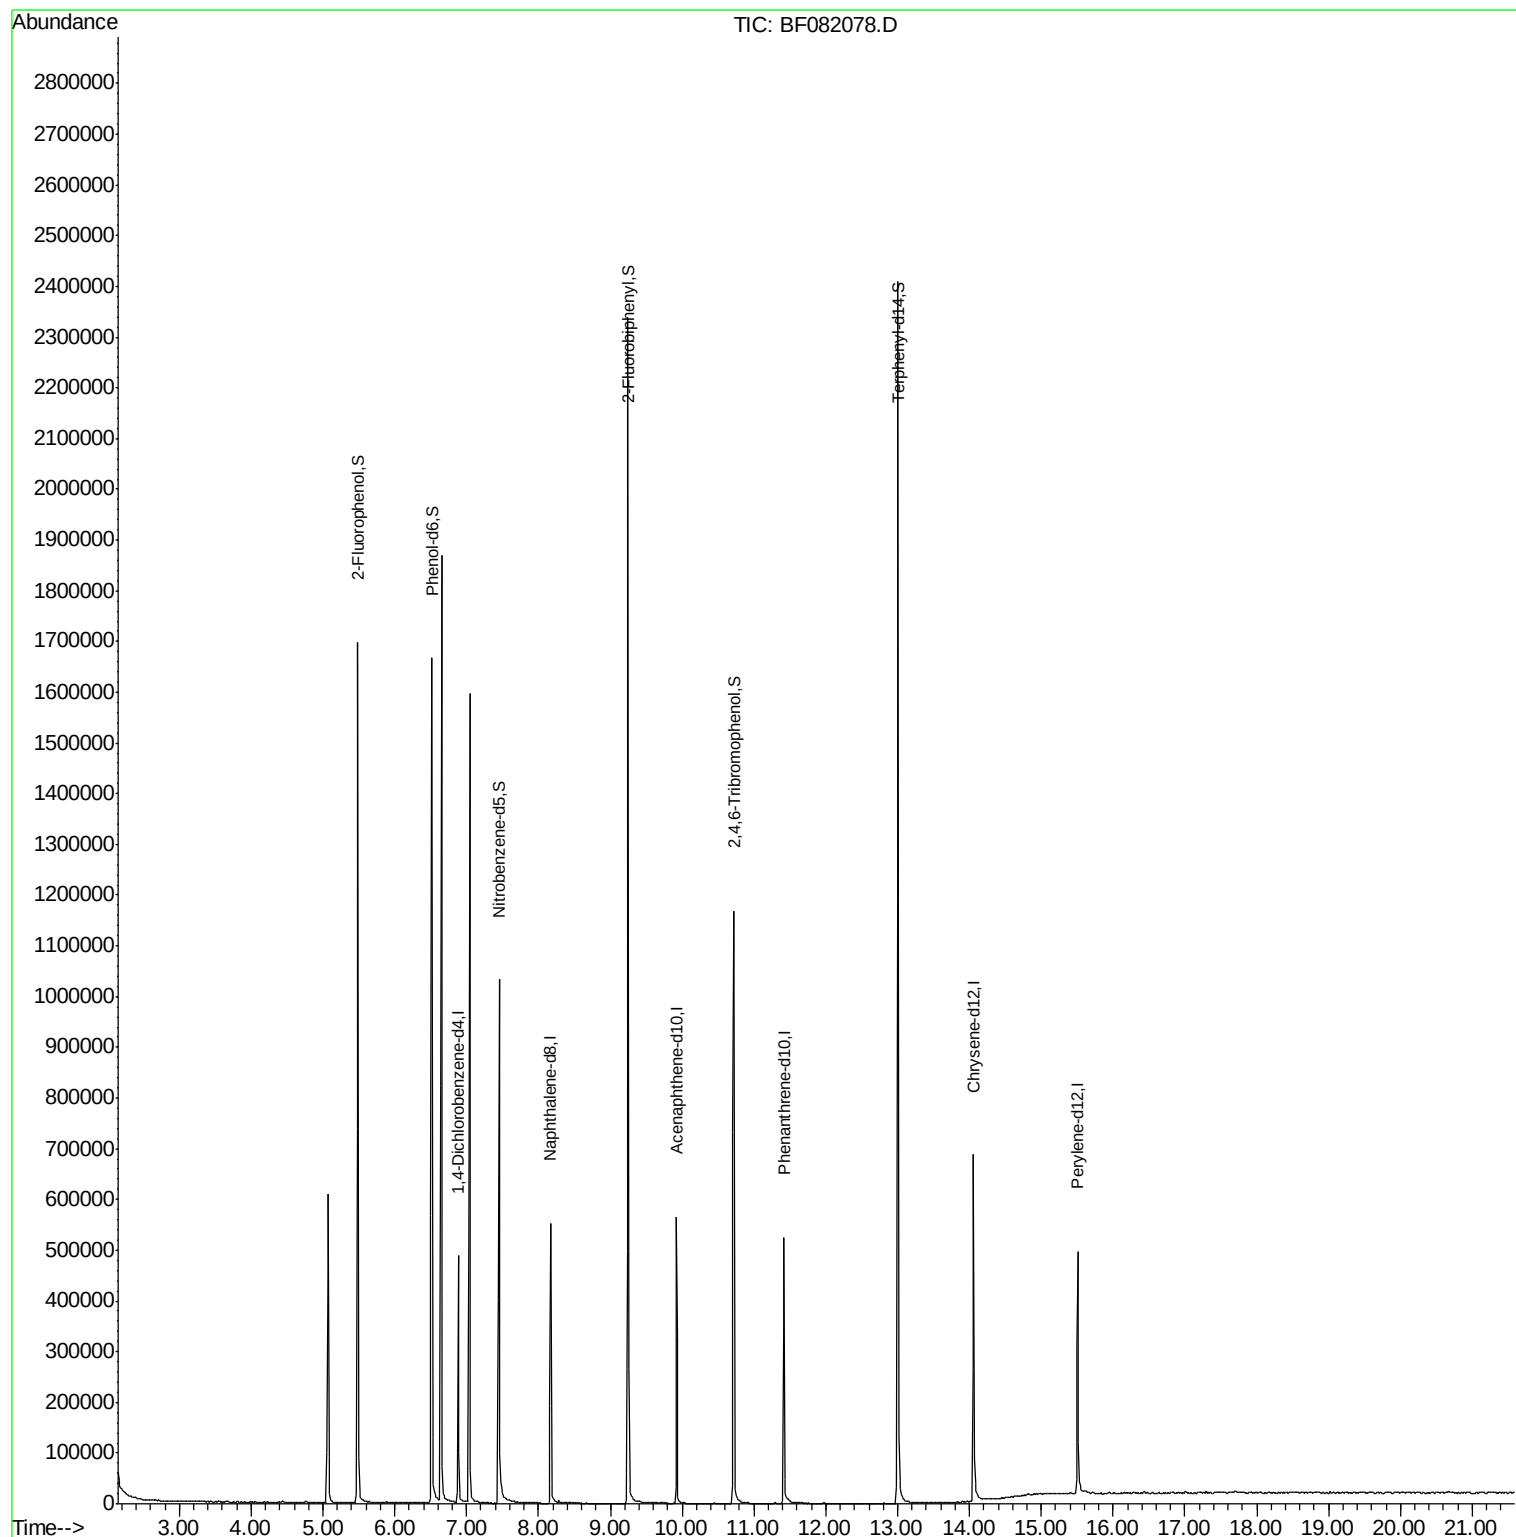

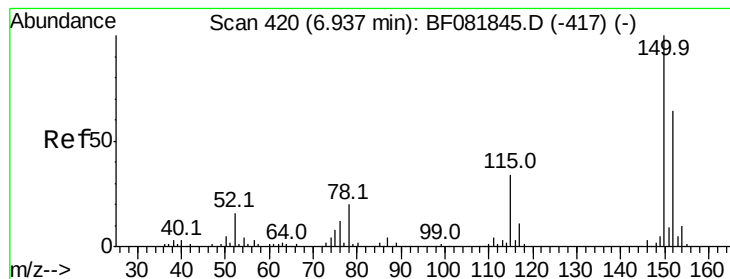

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.88 min Scan# 415

Delta R.T. 0.00 min

Lab File: BF082078.D

Acq: 6 Oct 2015 12:04

Instrument :

BNA_F

ClientSampleId :

PB85739BL


Tot Ion:152 Resp: 80847

Ion Ratio Lower Upper

152 100

150 159.5 124.7 187.1




115 60.6 39.0 58.4#

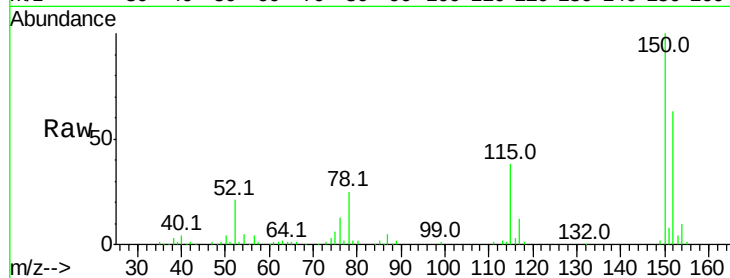

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

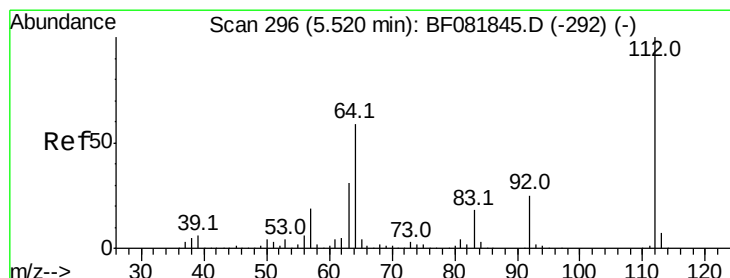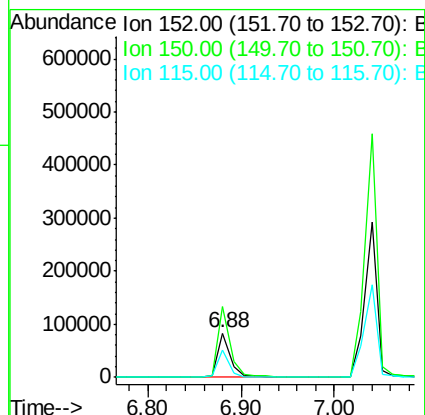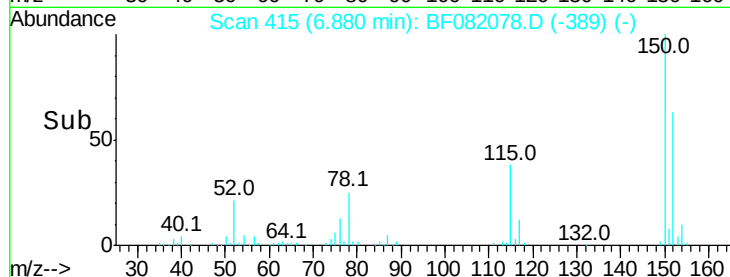

#5

2-Fluorophenol

Concen: 114.28 ng

RT: 5.49 min Scan# 293

Delta R.T. 0.01 min

Lab File: BF082078.D

Acq: 6 Oct 2015 12:04


Tgt Ion:112 Resp: 508972

Ion Ratio Lower Upper

112 100

64 60.5 39.7 59.5#



63 31.7 17.4 26.0#

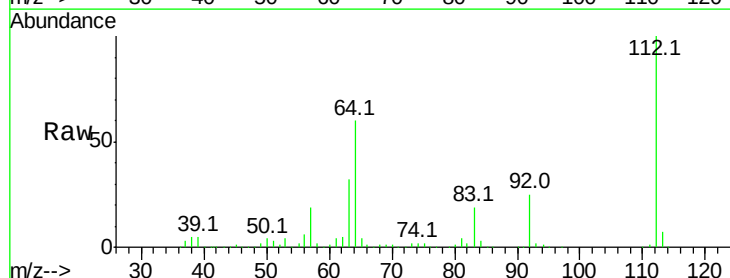


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

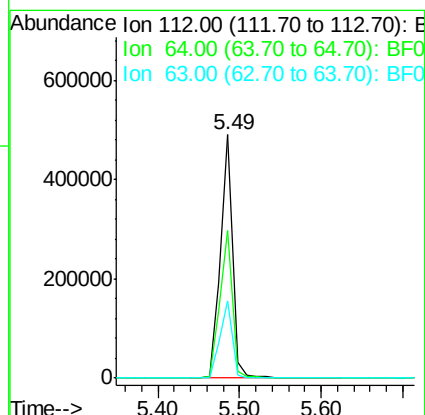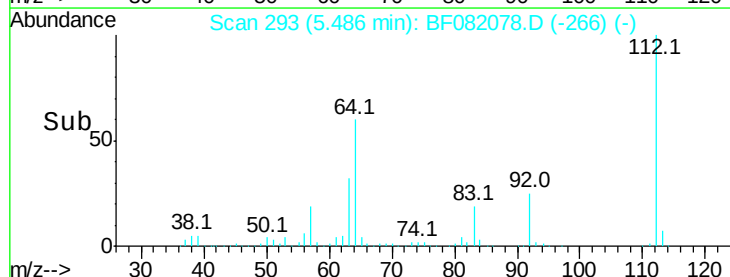

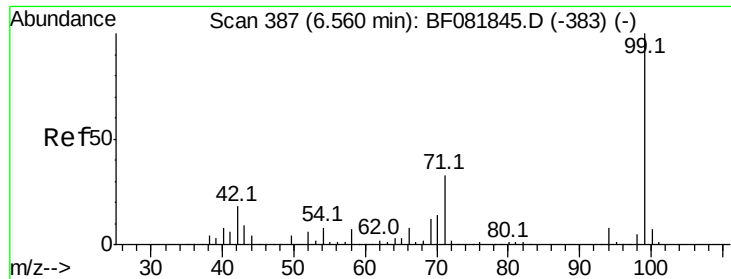

#7

Phenol-d6

Concen: 113.17 ng

RT: 6.51 min Scan# 383

Delta R.T. 0.00 min

Lab File: BF082078.D

Acq: 6 Oct 2015 12:04

Instrument :

BNA_F

ClientSampleId :

PB85739BL


Tot Ion: 99 Resp: 634231

Ion Ratio Lower Upper

99 100

42 18.1 13.7 20.5




71 34.7 14.2 21.2#

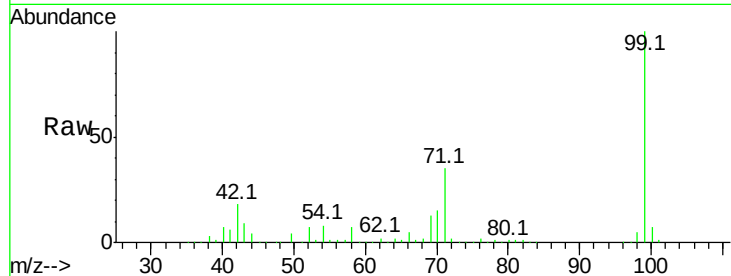

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

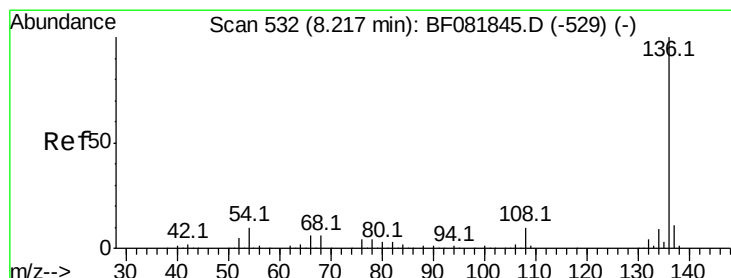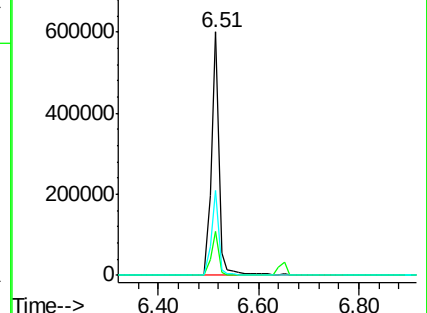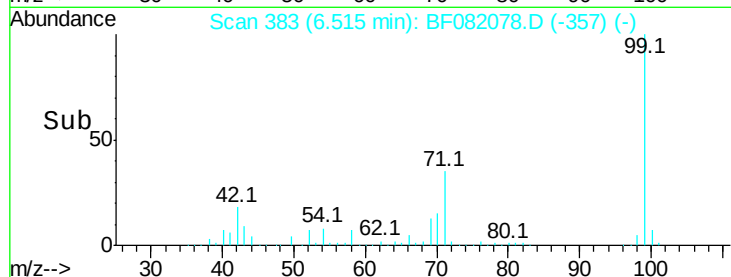

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.17 min Scan# 528

Delta R.T. 0.00 min

Lab File: BF082078.D

Acq: 6 Oct 2015 12:04

Tgt Ion: 136 Resp: 309301


Ion Ratio Lower Upper

136 100

137 10.8 9.0 13.6

54 6.5 8.2 12.2#

68 4.3 5.8 8.6#


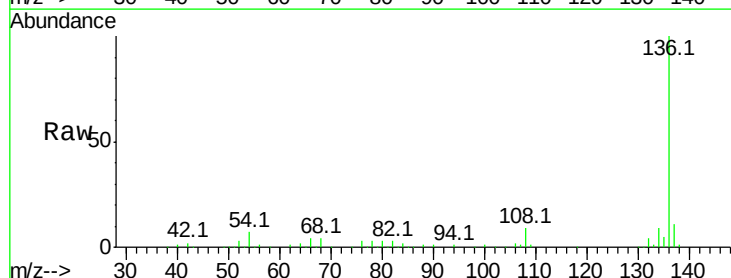



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

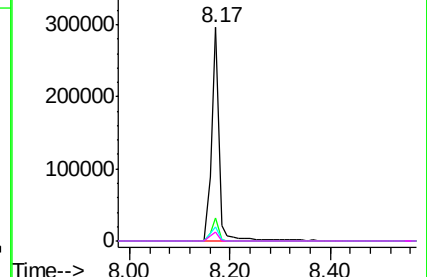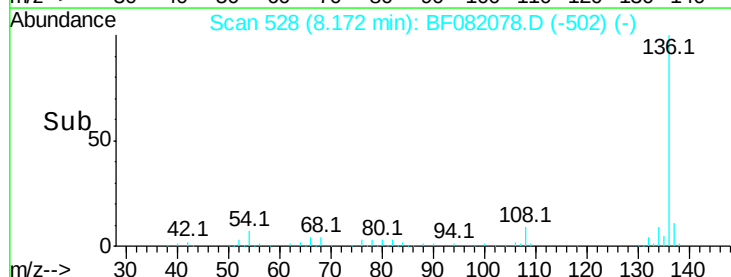

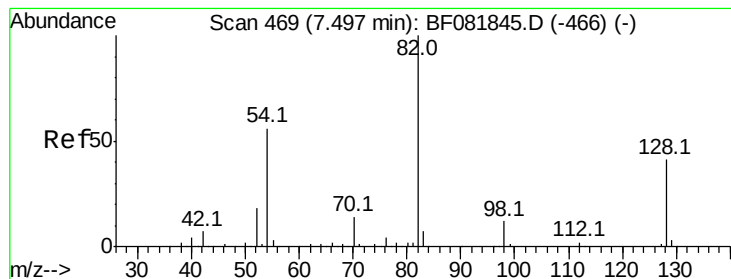

#23

Nitrobenzene-d5

Concen: 90.11 ng

RT: 7.45 min Scan# 465

Delta R.T. 0.00 min

Lab File: BF082078.D

Acq: 6 Oct 2015 12:04

Instrument :

BNA_F

ClientSampleId :

PB85739BL


Tot Ion: 82 Resp: 418112

Ion Ratio Lower Upper




82 100

128 46.2 51.0 76.6#

54 50.6 47.5 71.3

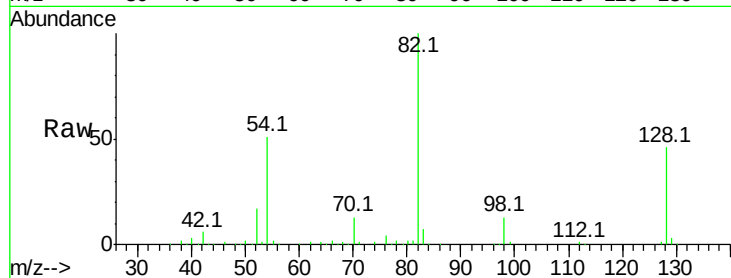

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

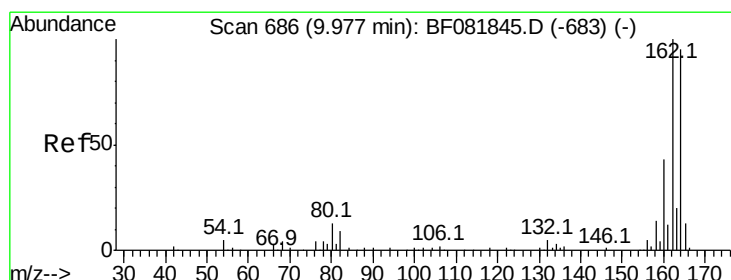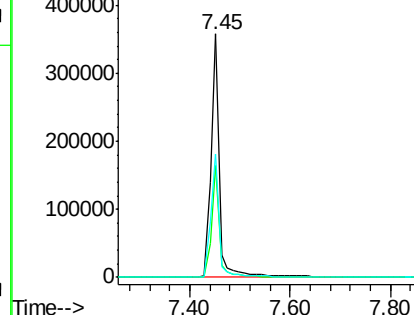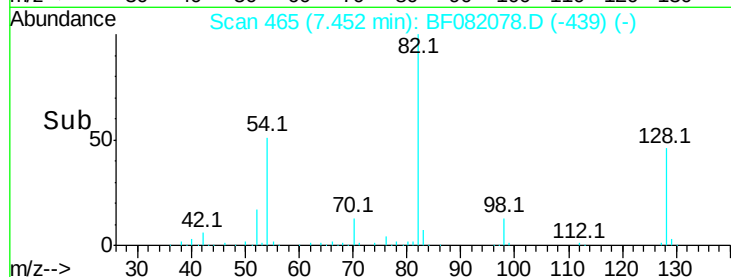

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.92 min Scan# 681

Delta R.T. -0.01 min

Lab File: BF082078.D

Acq: 6 Oct 2015 12:04


Tgt Ion:164 Resp: 146428

Ion Ratio Lower Upper



164 100


162 102.2 75.2 112.8

160 44.3 31.5 47.3

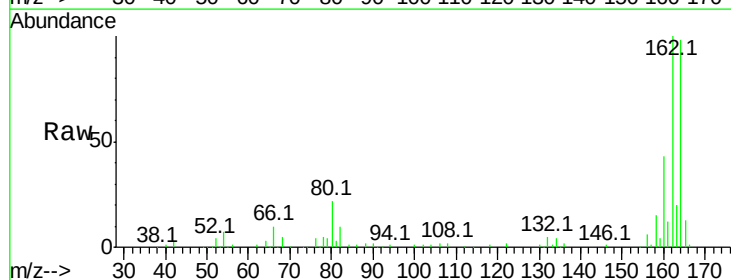

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

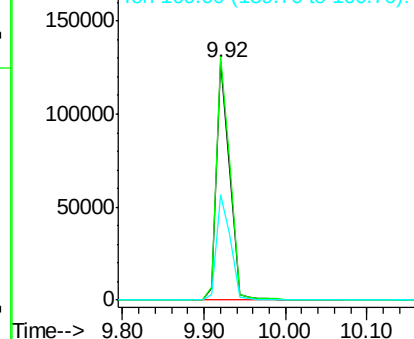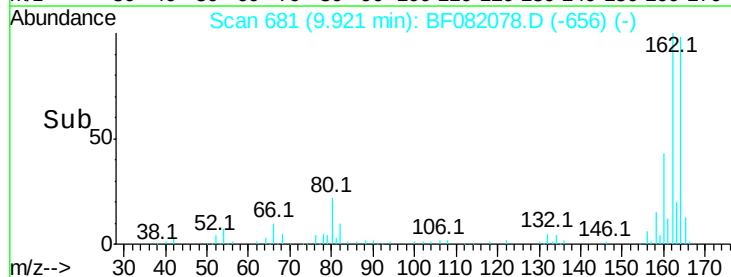


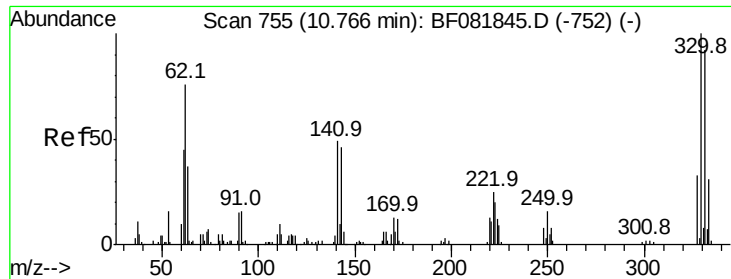




#41
 2,4,6-Tribromophenol
 Concen: 133.76 ng
 RT: 10.72 min Scan# 751
 Delta R.T. 0.00 min
 Lab File: BF082078.D
 Acq: 6 Oct 2015 12:04

Instrument :
 BNA_F
 ClientSampleId :
 PB85739BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.0	76.6	114.8
141	32.3	29.7	44.5

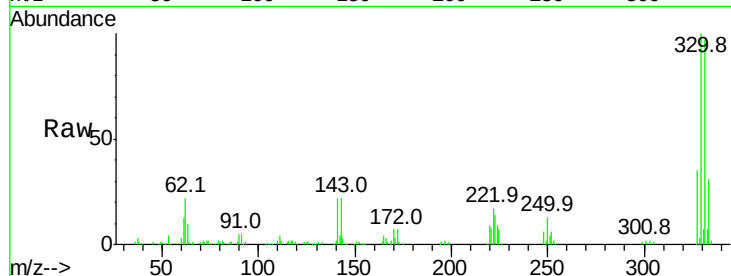


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

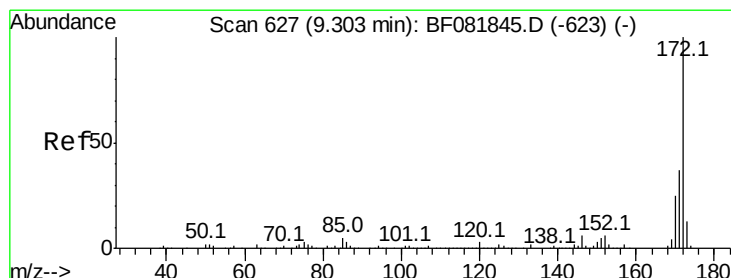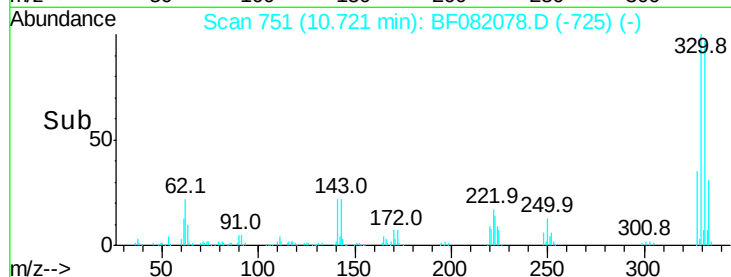
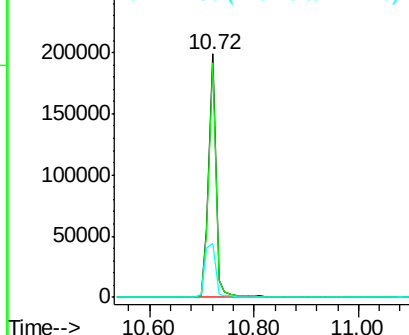



#44
 2-Fluorobiphenyl
 Concen: 91.91 ng
 RT: 9.25 min Scan# 622
 Delta R.T. 0.00 min
 Lab File: BF082078.D
 Acq: 6 Oct 2015 12:04

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.9	26.1	39.1
170	24.4	17.4	26.2

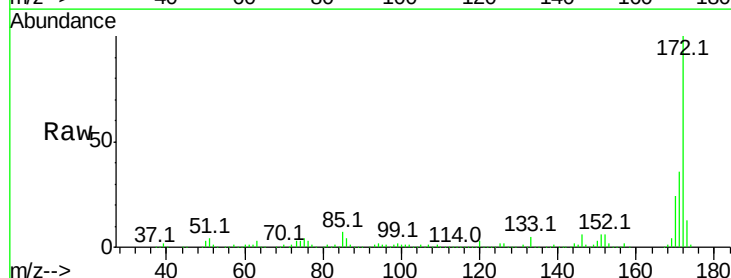

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



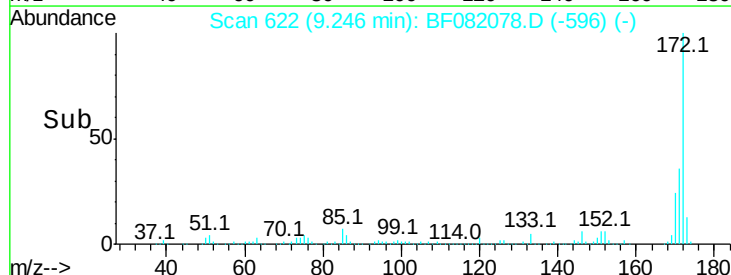
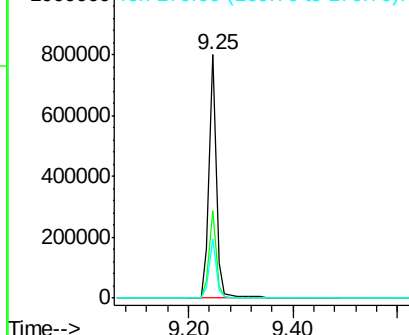


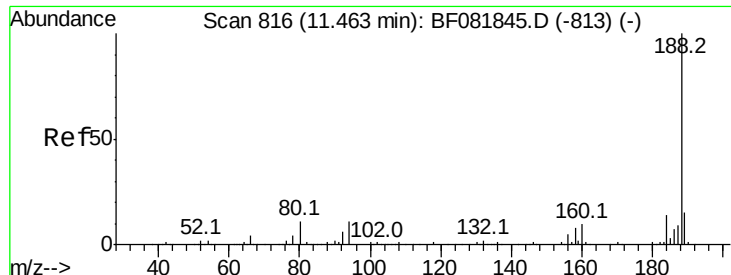

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.42 min Scan# 812
Delta R.T. 0.00 min
Lab File: BF082078.D
Acq: 6 Oct 2015 12:04




Instrument :
BNA_F
ClientSampleId :
PB85739BL


Tot Ion:188 Resp: 307012
Ion Ratio Lower Upper
188 100
94 5.8 11.1 16.7#
80 6.1 11.0 16.4#

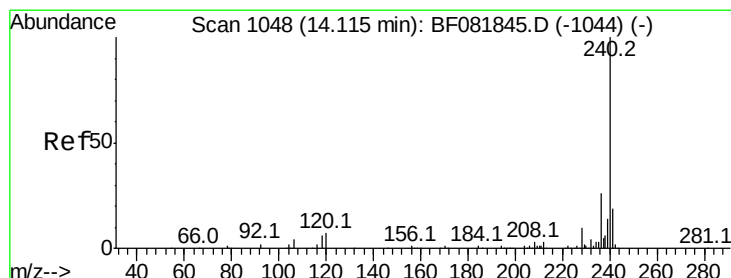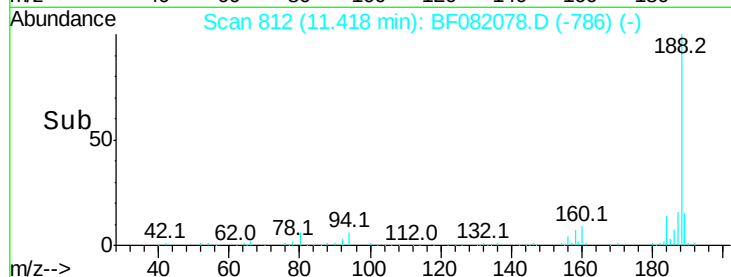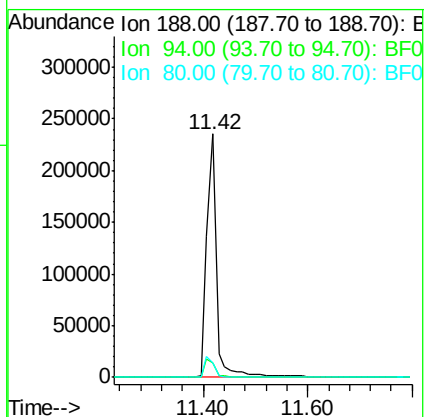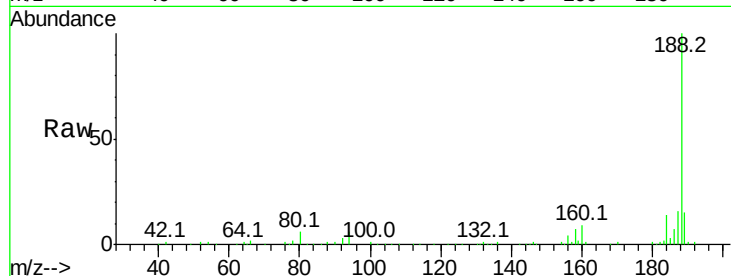

#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.06 min Scan# 1043
Delta R.T. -0.01 min
Lab File: BF082078.D
Acq: 6 Oct 2015 12:04

Tgt Ion:240 Resp: 316470
Ion Ratio Lower Upper
240 100
120 7.9 16.2 24.2#
236 26.0 18.4 27.6

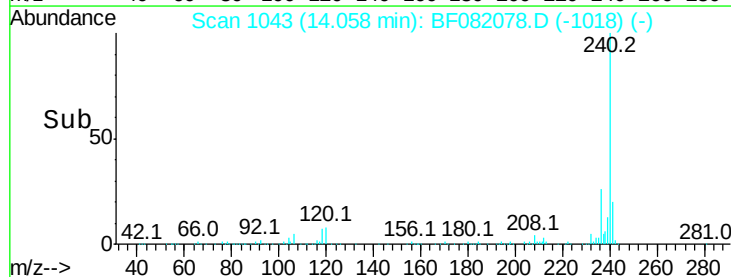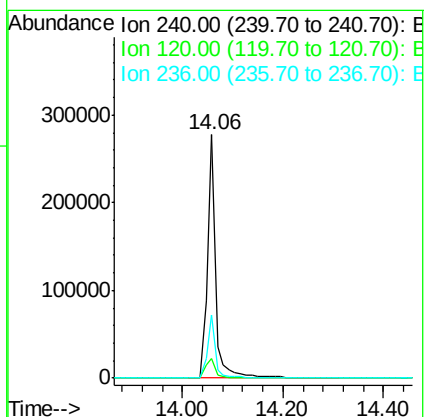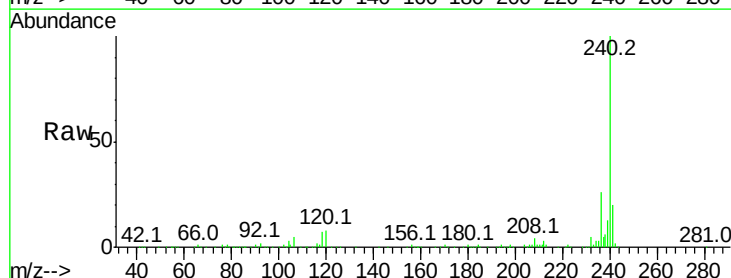


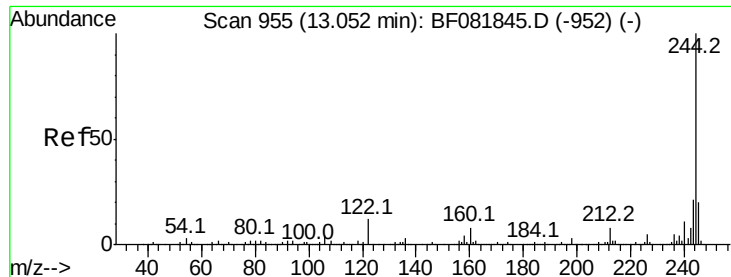




#78
 Terphenyl-d14
 Concen: 103.66 ng
 RT: 13.01 min Scan# 951
 Delta R.T. 0.00 min
 Lab File: BF082078.D
 Acq: 6 Oct 2015 12:04

Instrument :
 BNA_F
 ClientSampleID :
 PB85739BL

Tot Ion:244 Resp: 955100
 Ion Ratio Lower Upper
 244 100
 212 7.3 4.3 6.5#
 122 8.3 17.4 26.2#

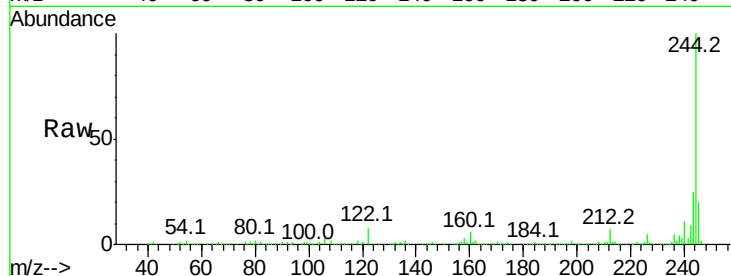


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

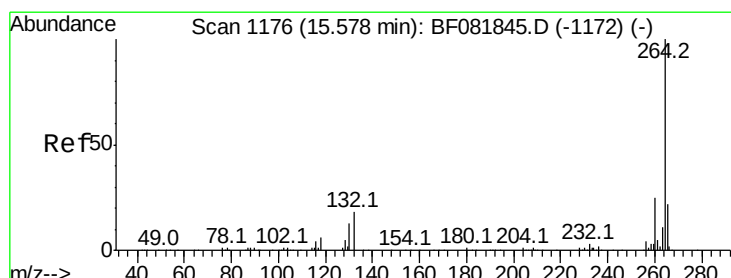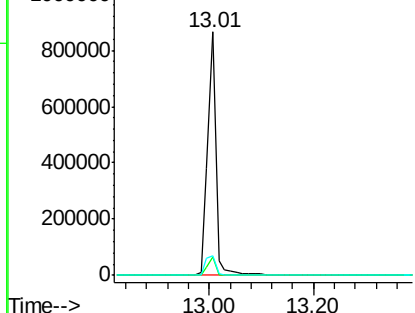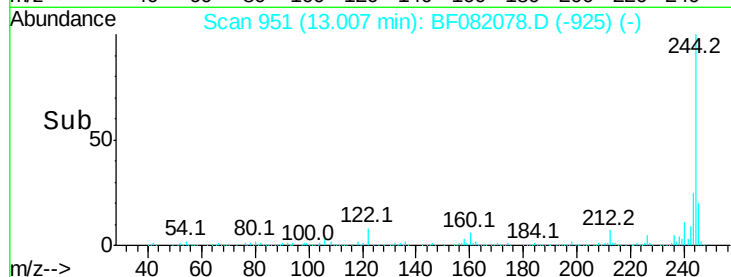

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.51 min Scan# 1170
 Delta R.T. 0.00 min
 Lab File: BF082078.D
 Acq: 6 Oct 2015 12:04

Tgt Ion:264 Resp: 264689
 Ion Ratio Lower Upper
 264 100
 260 23.7 16.7 25.1
 265 21.1 17.2 25.8

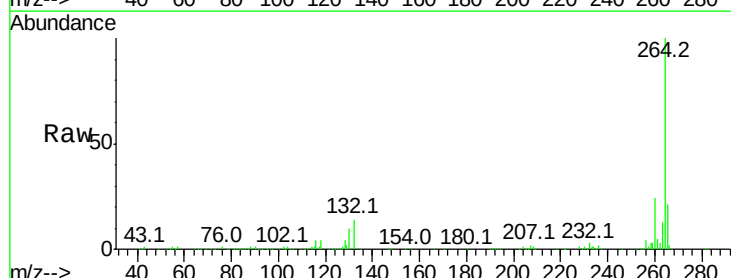

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

