


Data Path : Z:\HPCHEM1\BNA F\DATA\BF100615\
 Data File : BF082076.D
 Acq On : 6 Oct 2015 11:01
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 05 17:58:12 2015

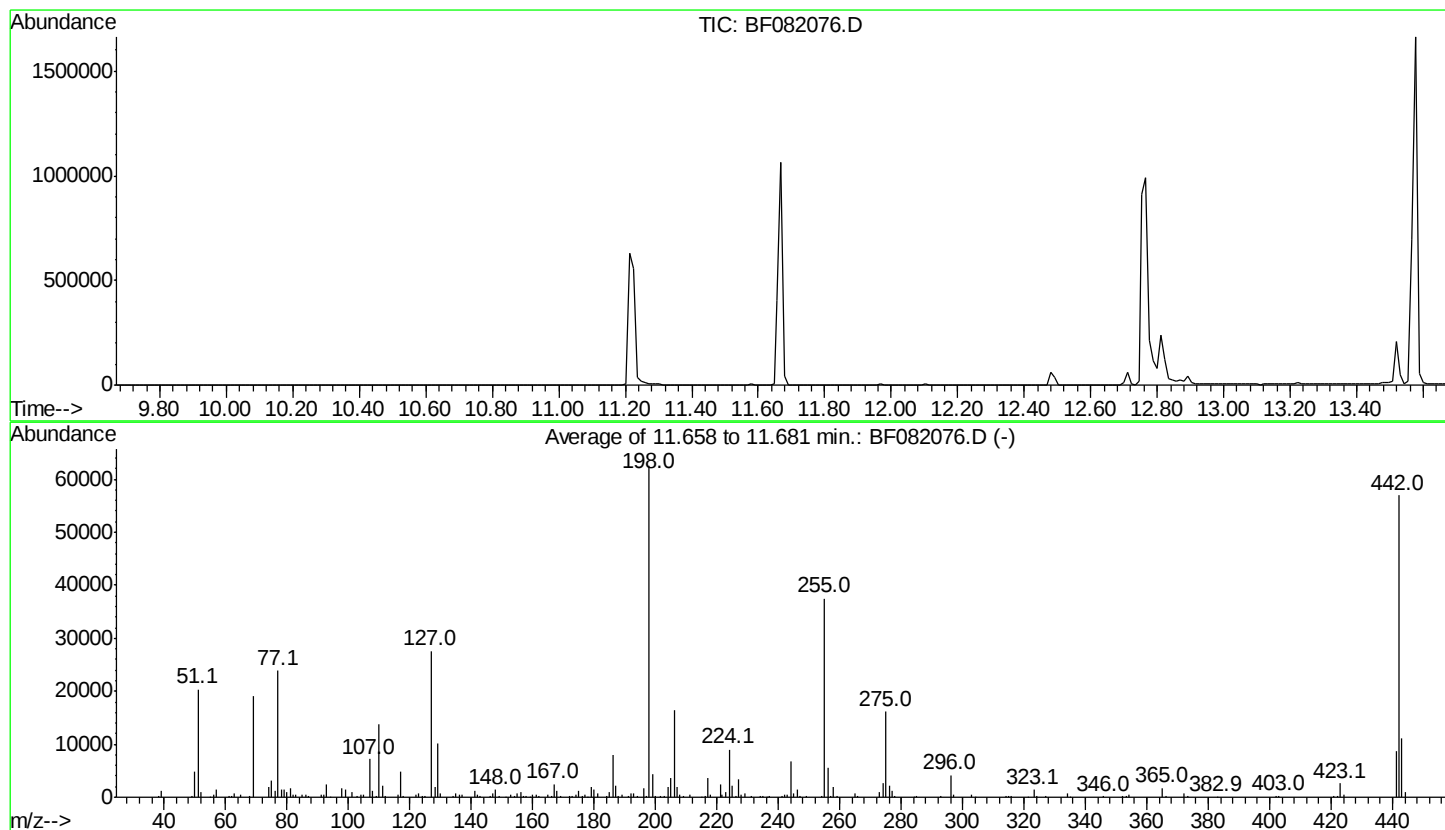

AutoFind: Scans 833, 834, 835; Background Corrected with Scan 829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	20376	PASS
68	69	0.00	2	1.5	295	PASS
69	198	0.00	100	30.4	19042	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.2	27661	PASS
197	198	0.00	2	0.4	258	PASS
198	198	100	100	100.0	62575	PASS
199	198	5	9	7.0	4366	PASS
275	198	10	60	25.7	16090	PASS
365	198	1	100	2.8	1731	PASS
441	442	0.01	24	15.4	8776	PASS
442	198	50	100	91.0	56923	PASS
443	442	15	24	19.6	11156	PASS