


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100616\
Data File : BF090422.D
Acq On : 6 Oct 2016 15:43
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF100516.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 05 14:57:00 2016

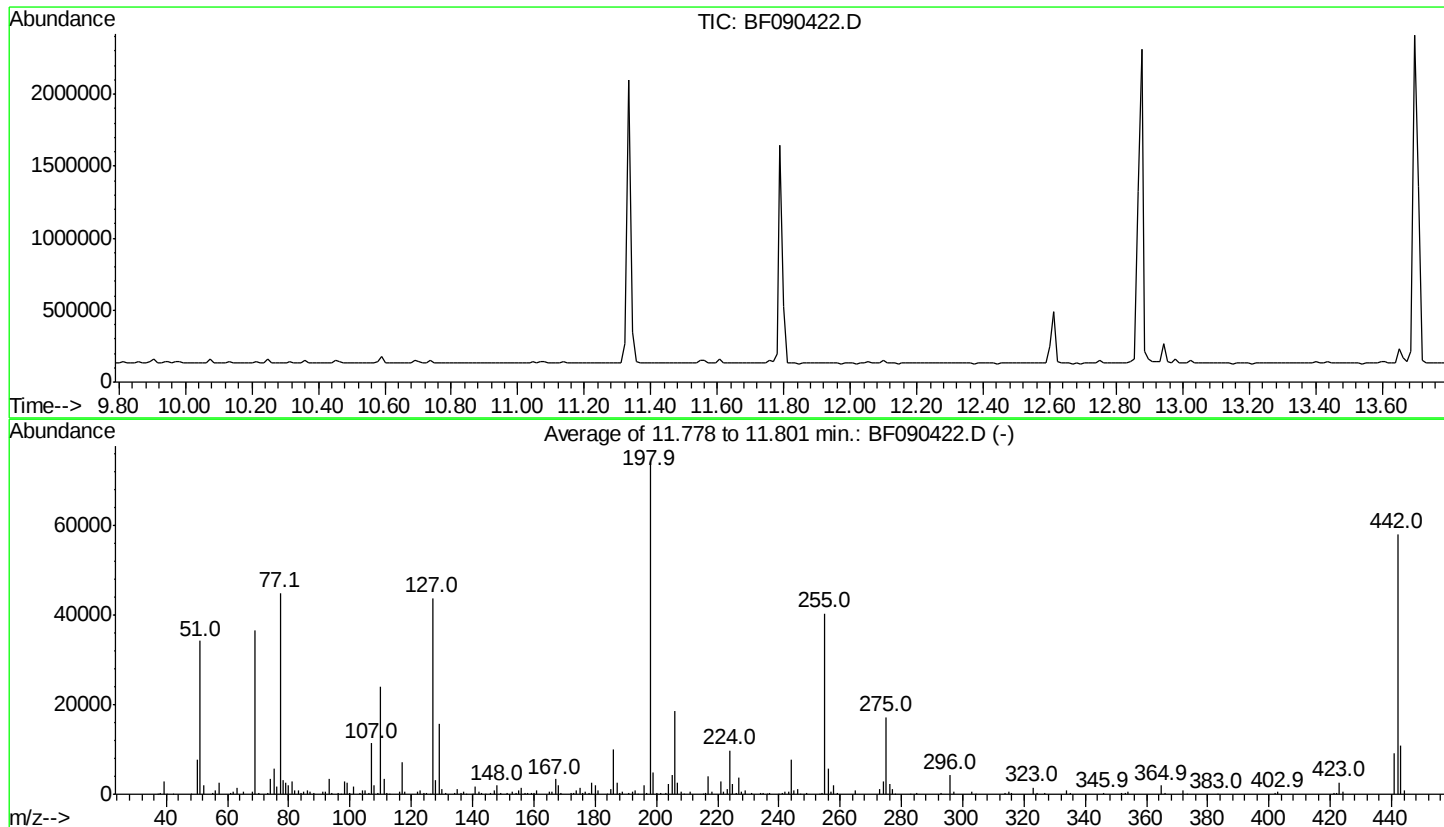

AutoFind: Scans 826, 827, 828; Background Corrected with Scan 823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	34283	PASS
68	69	0.00	2	1.3	472	PASS
69	198	0.00	100	49.4	36593	PASS
70	69	0.00	2	1.1	398	PASS
127	198	10	80	59.1	43767	PASS
197	198	0.00	2	0.3	238	PASS
198	198	100	100	100.0	74064	PASS
199	198	5	9	6.8	5006	PASS
275	198	10	60	23.3	17275	PASS
365	198	1	100	2.6	1956	PASS
441	442	0.01	24	15.6	9071	PASS
442	198	50	100	78.5	58133	PASS
443	442	15	24	18.6	10813	PASS