
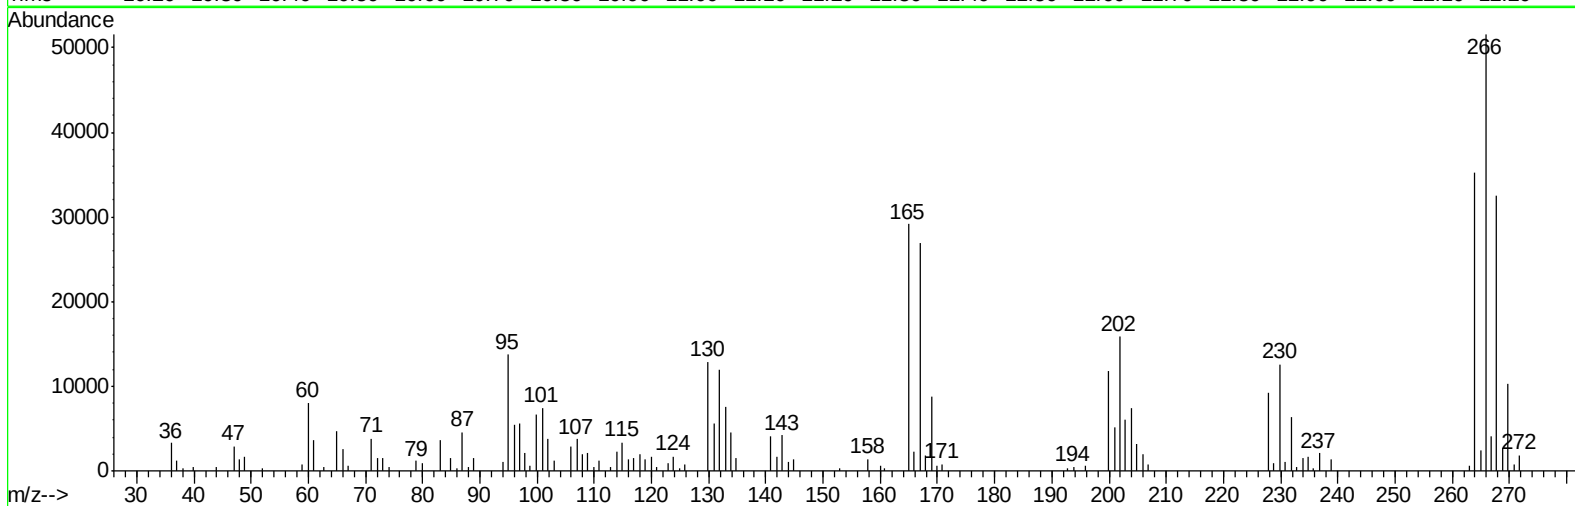


Data Path : Z:\HPCHEM1\BNA F\DATA\BF100617\
Data File : BF099137.D
Acq On : 6 Oct 2017 9:44
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 05:23:02 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 05 17:20:48 2017
Response via : Initial Calibration

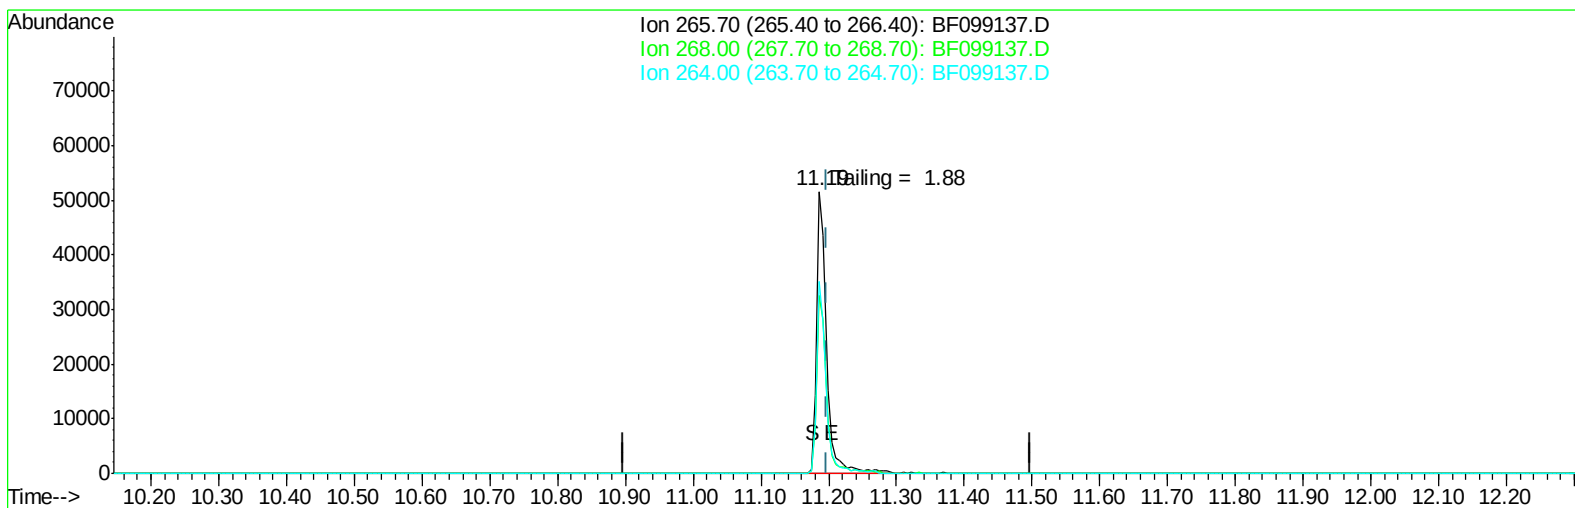

TIC: BF099137.D

(69) Pentachlorophenol (C)



11.186min (-0.012) 29379.78ng

response 51421

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.09
264.00	61.90	68.37
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100617\
Data File : BF099137.D
Acq On : 6 Oct 2017 9:44
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 05:23:02 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 05 17:20:48 2017
Response via : Initial Calibration

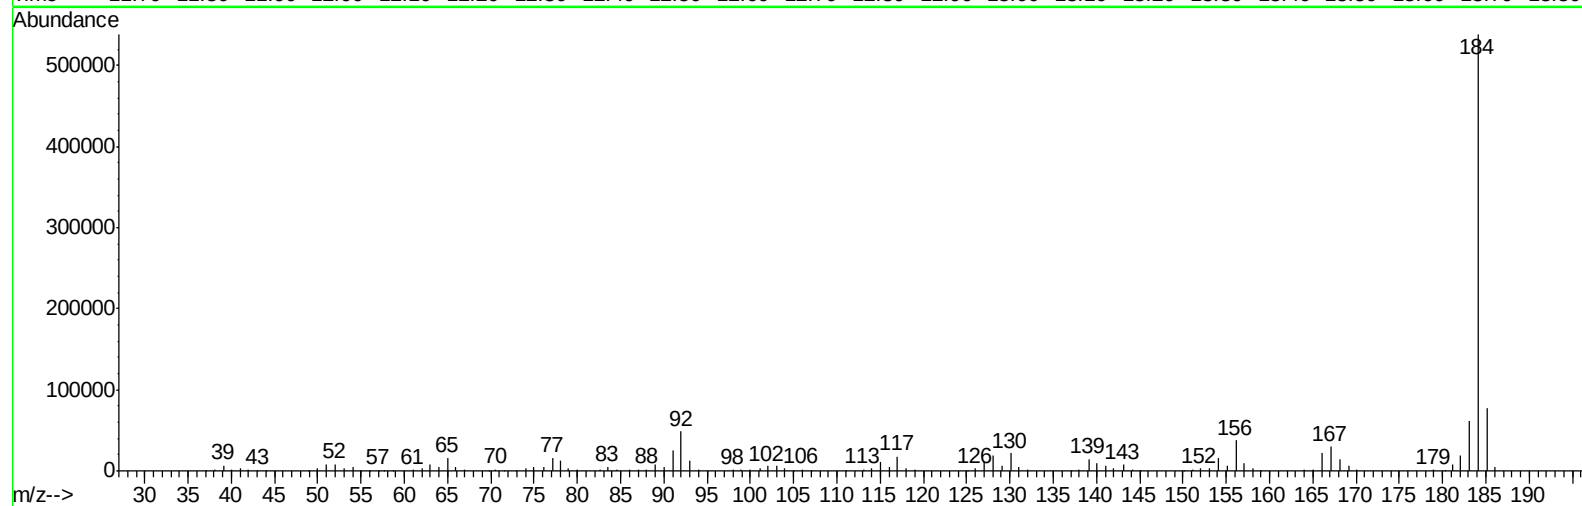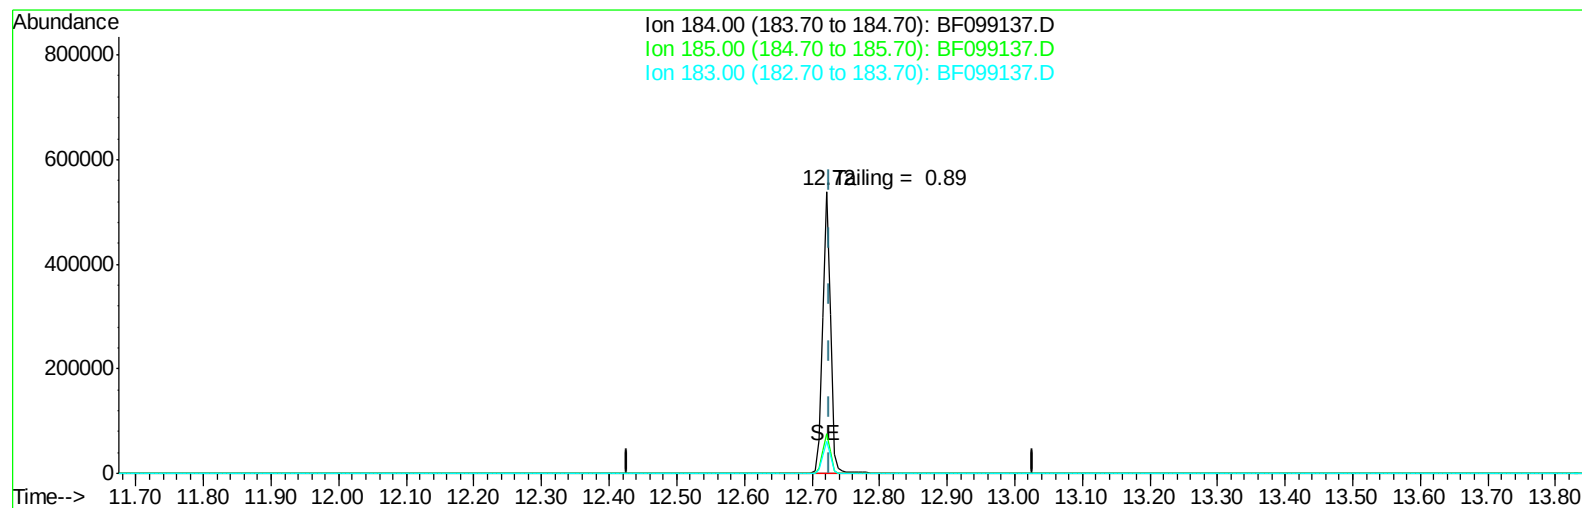

TIC: BF099137.D

(76) Benzidine

12.722min (-0.006) 0.00ng

response 451040

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.32
183.00	11.60	11.59
0.00	0.00	0.00