
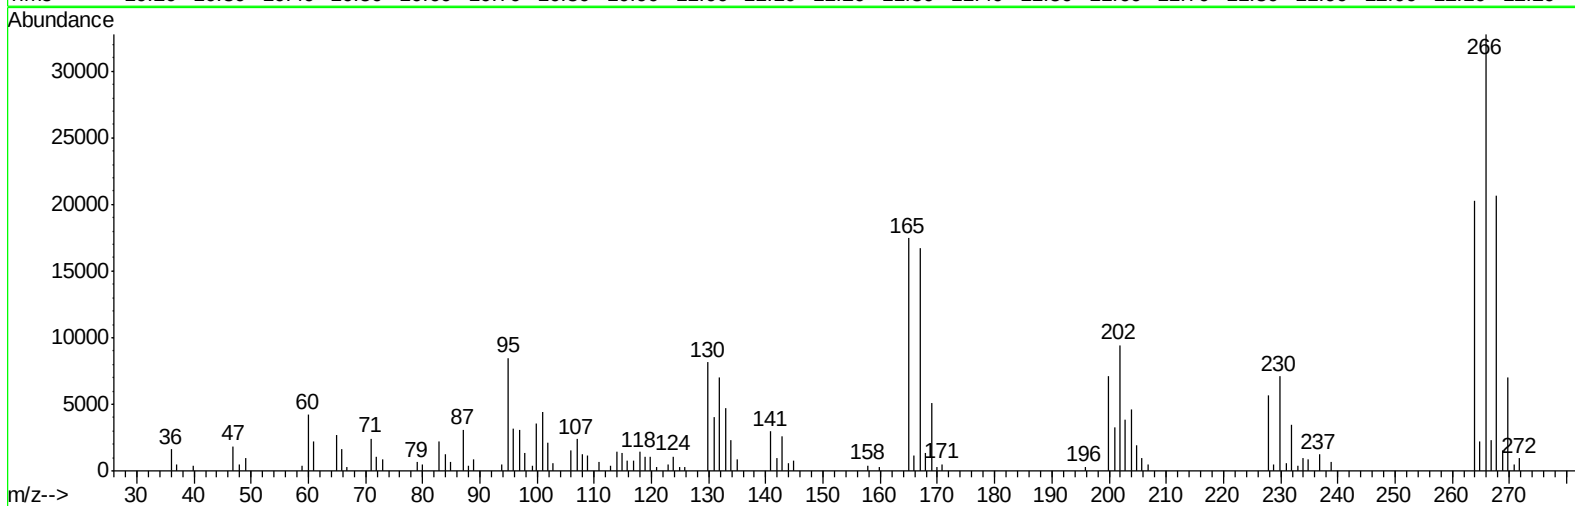


Data Path : Z:\HPCHEM1\BNA F\DATA\BF100617\
Data File : BF099173.D
Acq On : 7 Oct 2017 3:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 05:27:29 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 05 17:20:48 2017
Response via : Initial Calibration

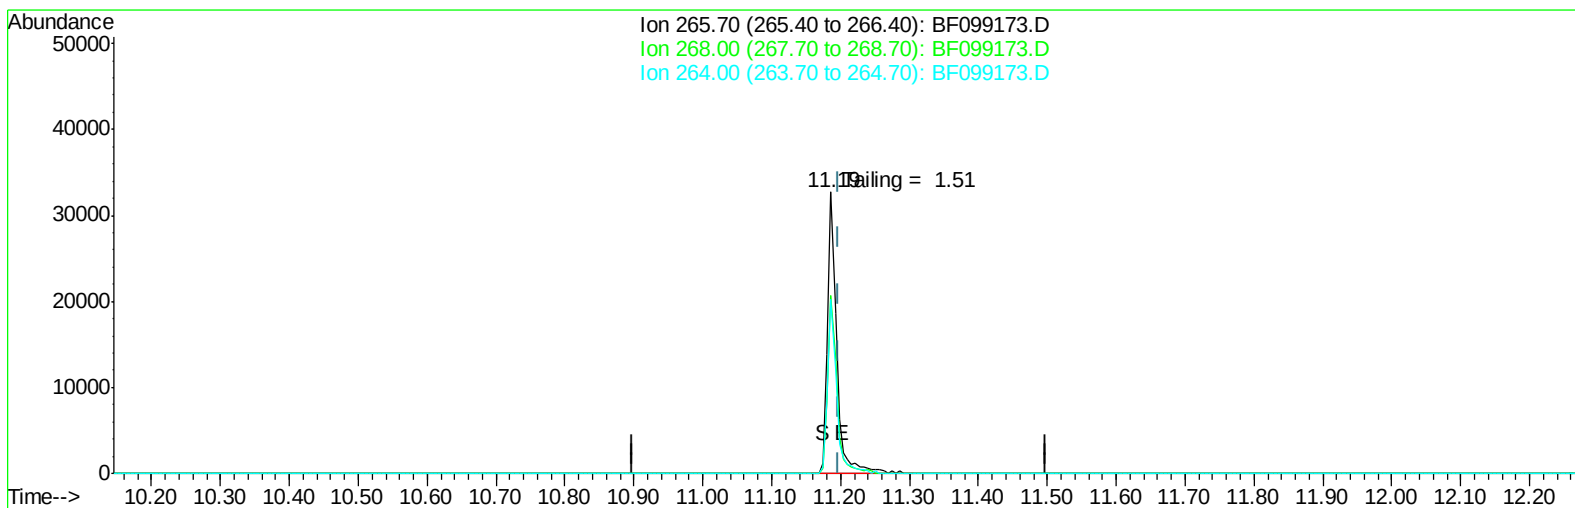

TIC: BF099173.D

(69) Pentachlorophenol (C)



11.186min (-0.012) 6113.84ng

response 29158

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.14
264.00	61.90	61.99
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100617\
Data File : BF099173.D
Acq On : 7 Oct 2017 3:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 05:27:29 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 05 17:20:48 2017
Response via : Initial Calibration

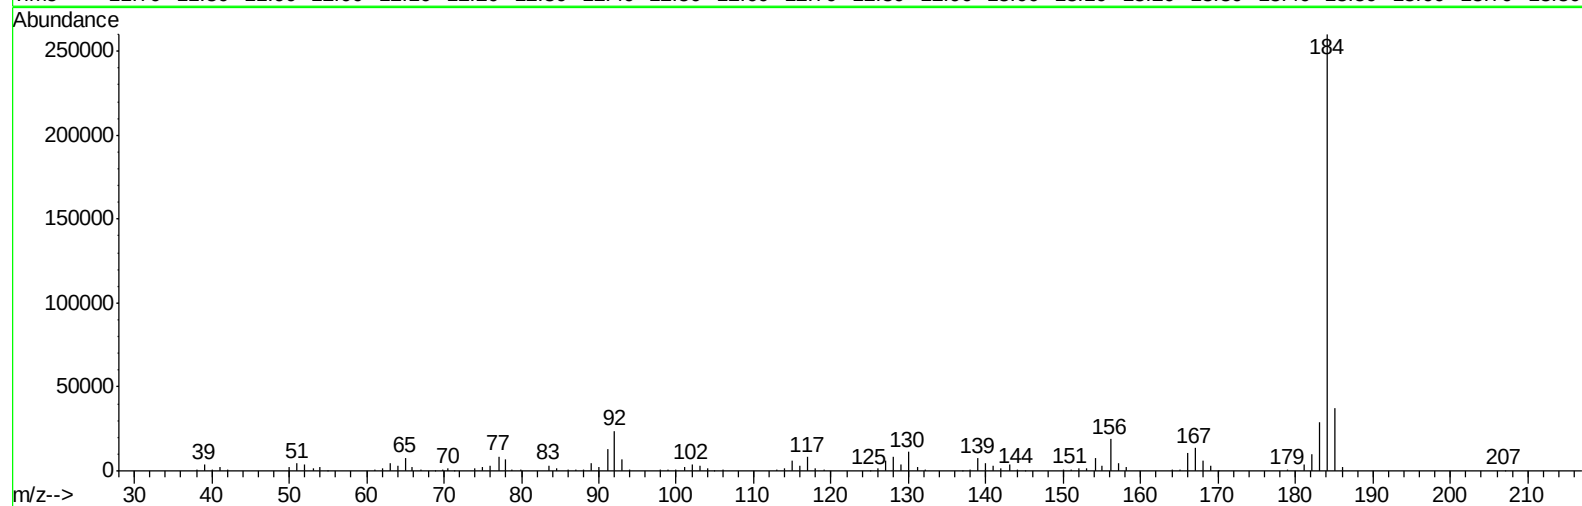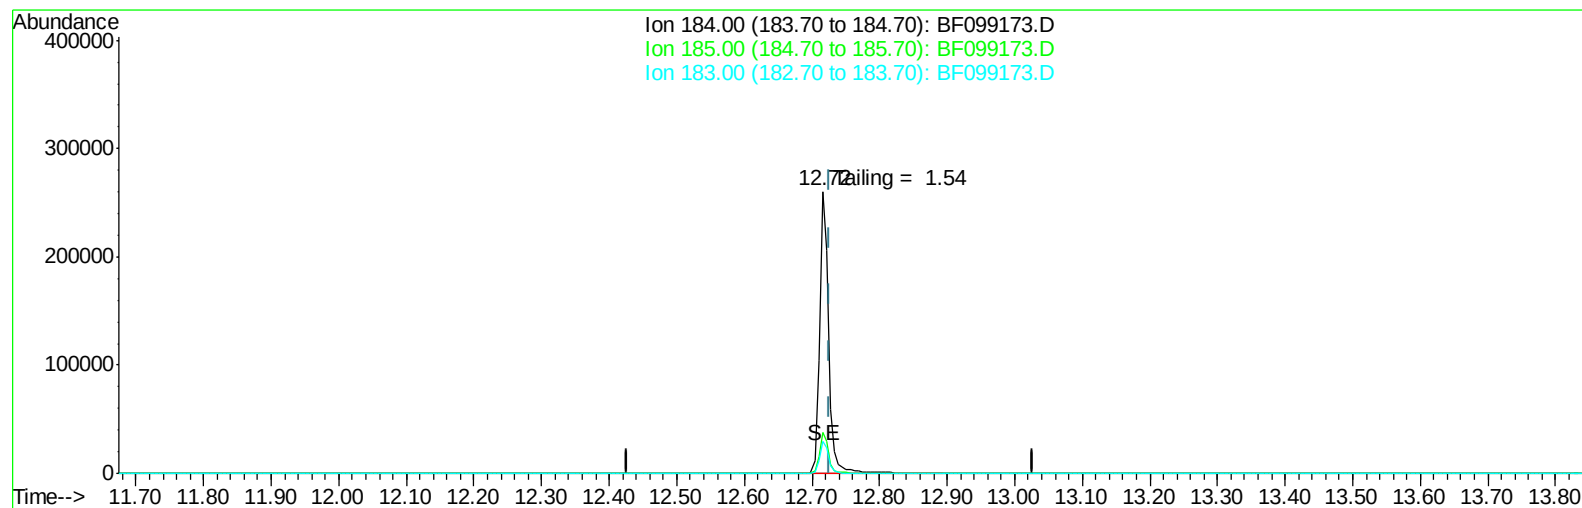

TIC: BF099173.D

(76) Benzidine

12.716min (-0.012) 19638.51ng

response 246236

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.42
183.00	11.60	11.22
0.00	0.00	0.00