

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100617\
 Data File : BF099153.D
 Acq On : 6 Oct 2017 17:56
 Operator : SJ/JU
 Sample : PB102940BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB102940BL

Quant Time: Oct 06 23:18:56 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 05 17:20:48 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	133454	20.00	ng	0.00
21) Naphthalene-d8	8.15	136	547765	20.00	ng	0.00
38) Acenaphthene-d10	9.90	164	249629	20.00	ng	0.00
63) Phenanthrene-d10	11.39	188	432602	20.00	ng	0.00
75) Chrysene-d12	14.02	240	301243	20.00	ng	-0.01
86) Perylene-d12	15.50	264	228209	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.49	112	951642	113.52	ng	0.01
7) Phenol-d6	6.50	99	1116304	107.94	ng	0.00
23) Nitrobenzene-d5	7.43	82	690764	80.87	ng	0.00
41) 2,4,6-Tribromophenol	10.69	330	233787	114.45	ng	0.00
44) 2-Fluorobiphenyl	9.22	172	1261091	84.34	ng	0.00
78) Terphenyl-d14	12.97	244	1074282	81.10	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100617\
Data File : BF099153.D
Acq On : 6 Oct 2017 17:56
Operator : SJ/JU
Sample : PB102940BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB102940BL

Quant Time: Oct 06 23:18:56 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 05 17:20:48 2017
Response via : Initial Calibration

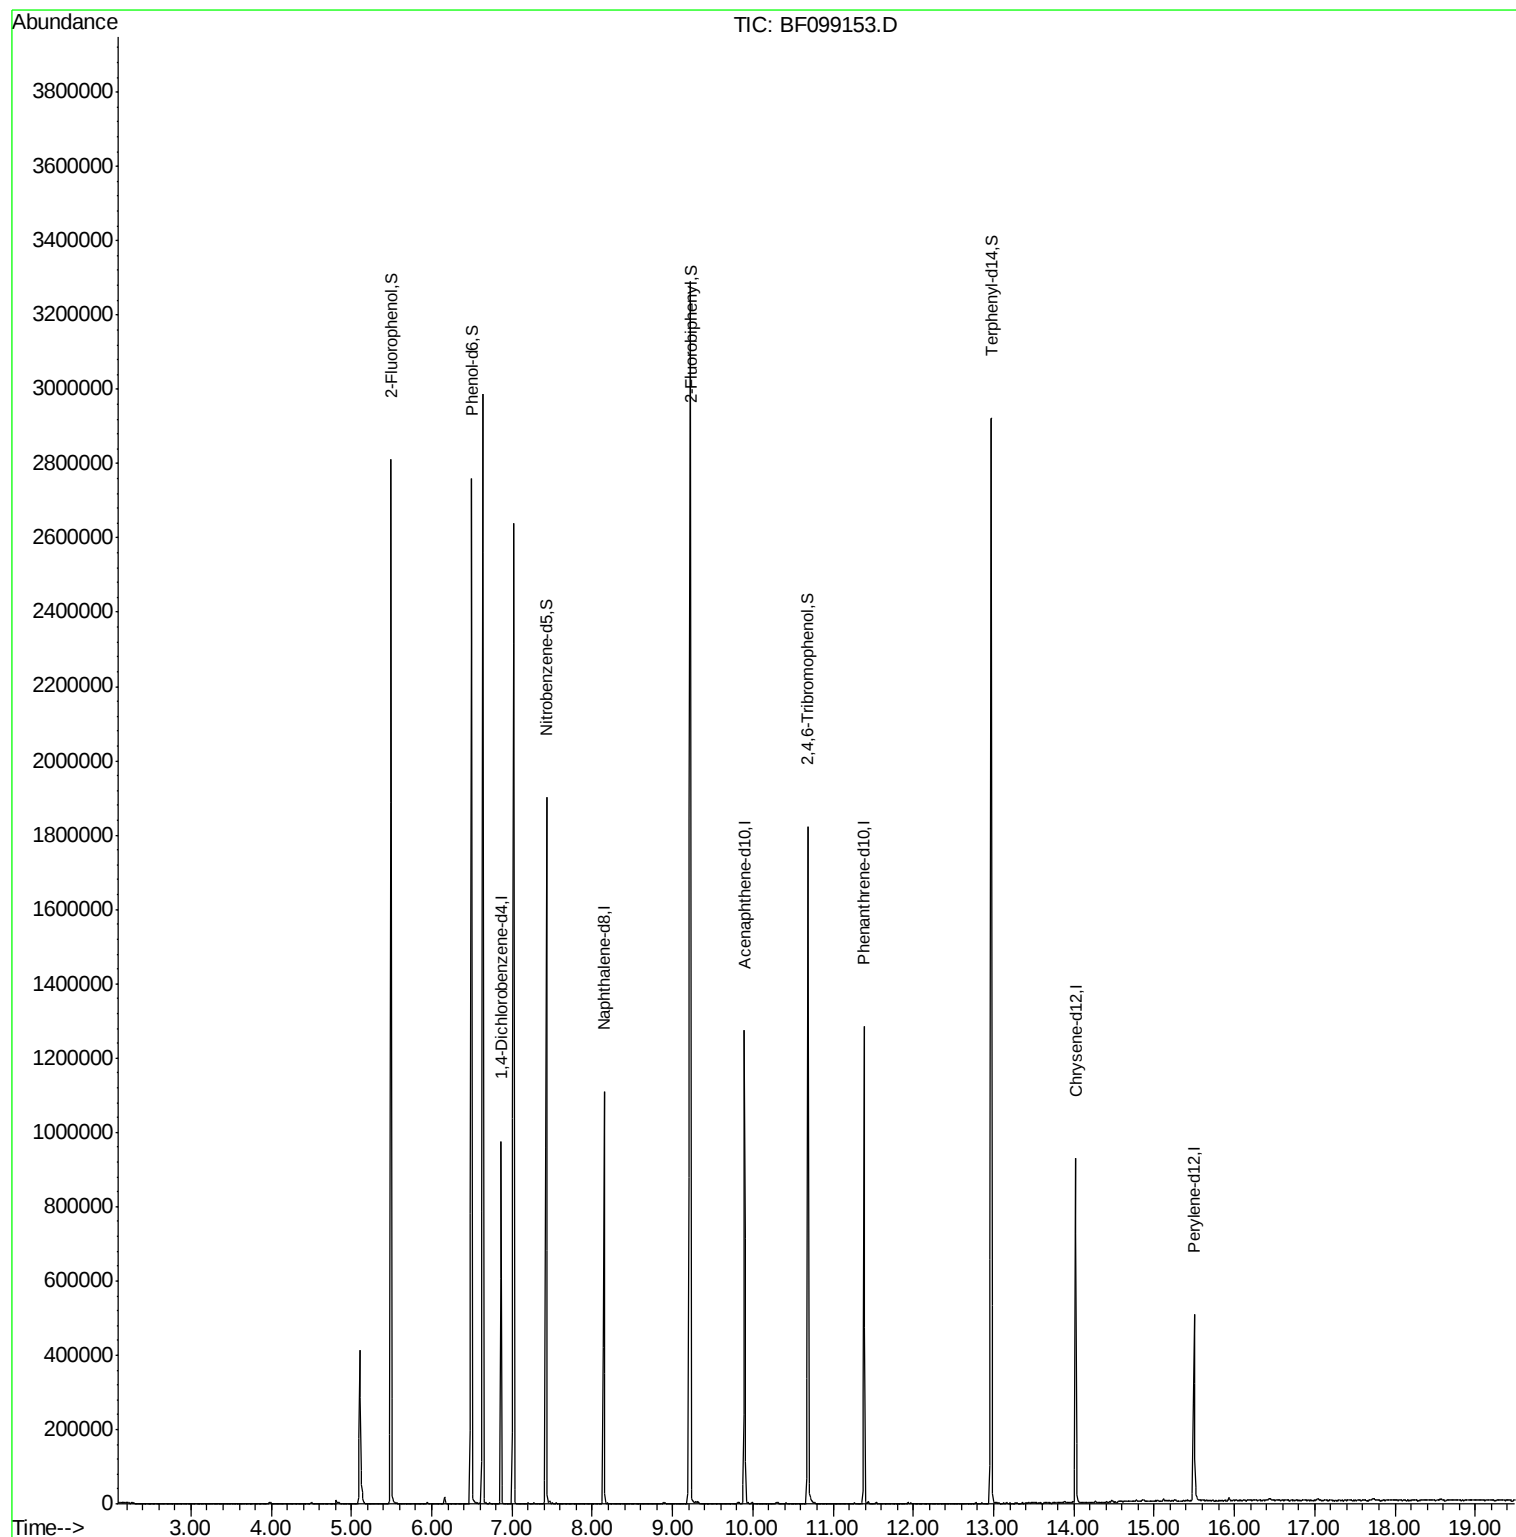

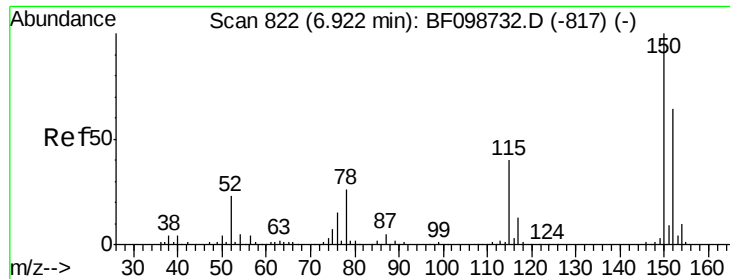

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.86 min Scan# 812

Delta R.T. -0.01 min

Lab File: BF099153.D

Acq: 6 Oct 2017 17:56

Instrument :

BNA_F

ClientSampleId :

PB102940BL


Tgt Ion:152 Resp: 133454

Ion Ratio Lower Upper

152 100

150 156.9 124.6 186.8




115 59.6 50.1 75.1

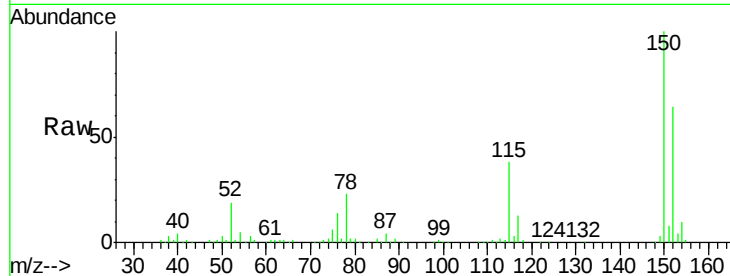

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

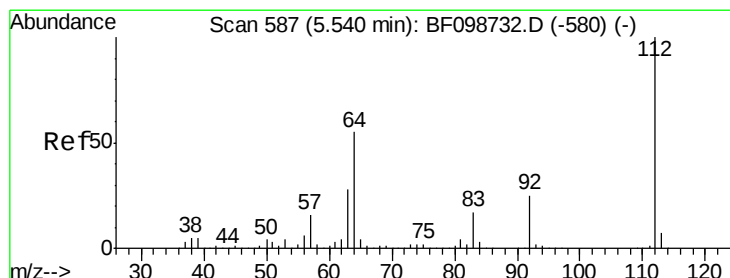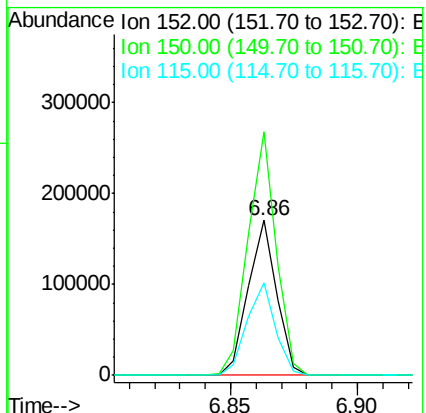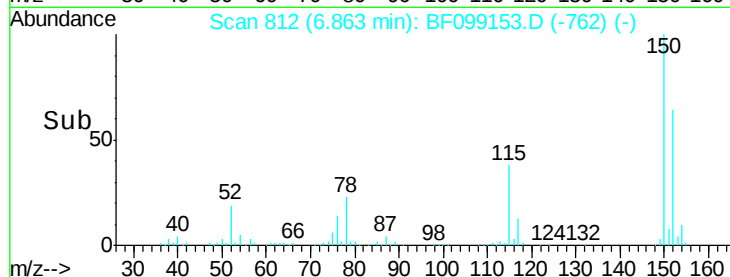

#5

2-Fluorophenol

Concen: 113.52 ng

RT: 5.49 min Scan# 579

Delta R.T. 0.01 min

Lab File: BF099153.D

Acq: 6 Oct 2017 17:56


Tgt Ion:112 Resp: 951642

Ion Ratio Lower Upper

112 100

64 57.2 47.9 71.9



63 27.9 23.7 35.5

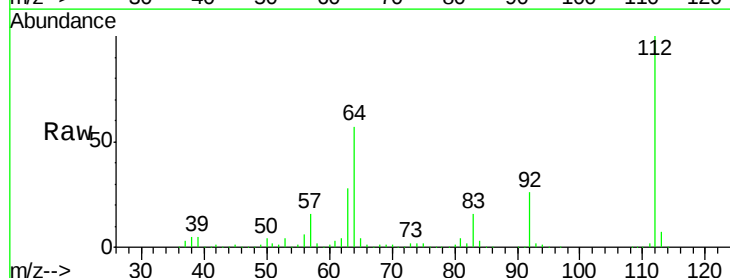

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

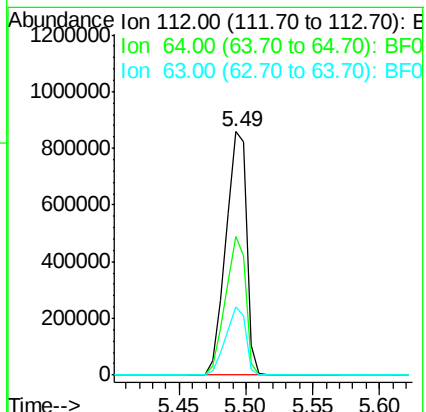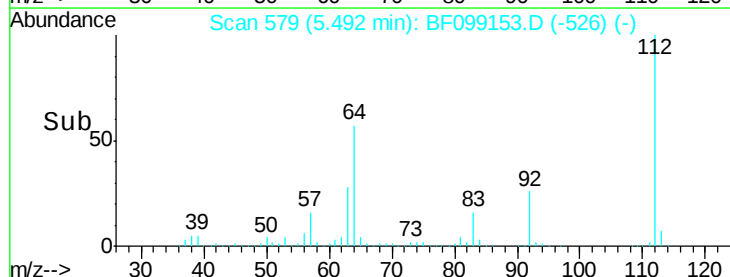



#7

Phenol-d6

Concen: 107.94 ng

RT: 6.50 min Scan# 750

Delta R.T. -0.00 min

Lab File: BF099153.D

Acq: 6 Oct 2017 17:56

Instrument :

BNA_F

ClientSampled :

PB102940BL


Tgt Ion: 99 Resp: 1116304

Ion Ratio Lower Upper

99 100

42 15.3 14.5 21.7




71 30.8 25.4 38.0

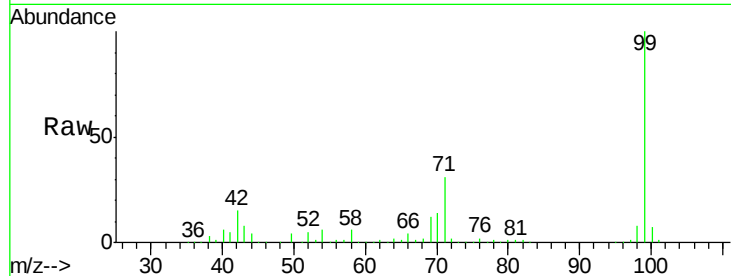

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

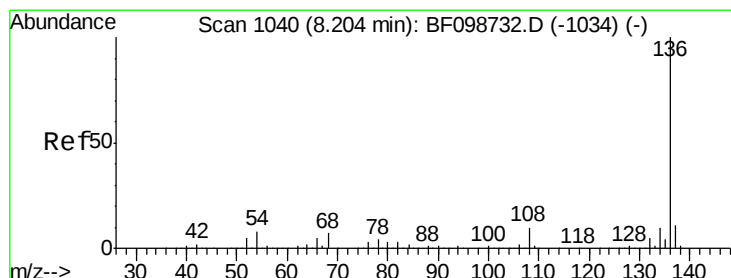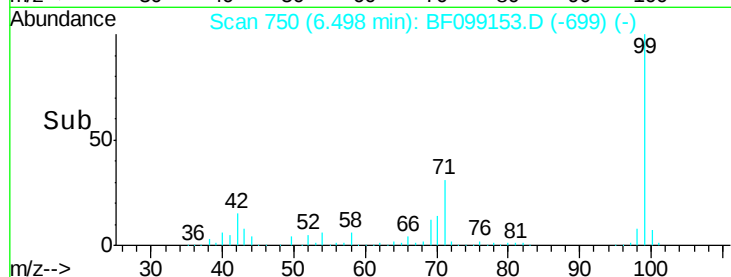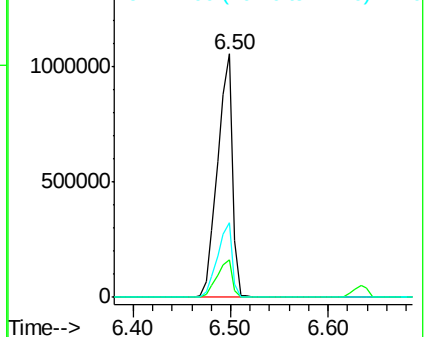

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.15 min Scan# 1030

Delta R.T. -0.01 min

Lab File: BF099153.D

Acq: 6 Oct 2017 17:56

Tgt Ion: 136 Resp: 547765


Ion Ratio Lower Upper

136 100

137 10.9 8.9 13.3

54 7.0 6.6 9.8

68 5.7 5.0 7.4


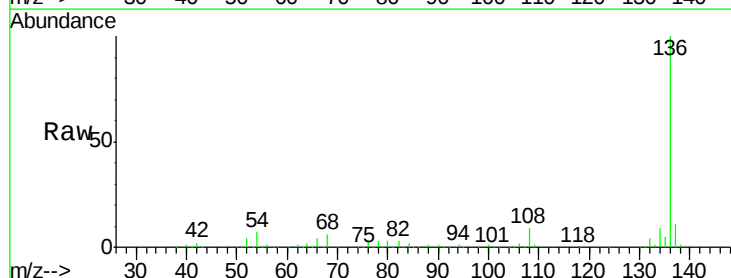



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

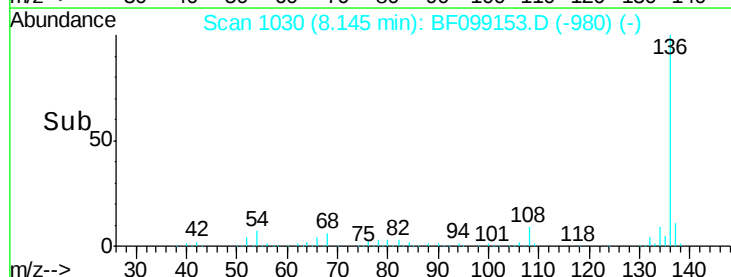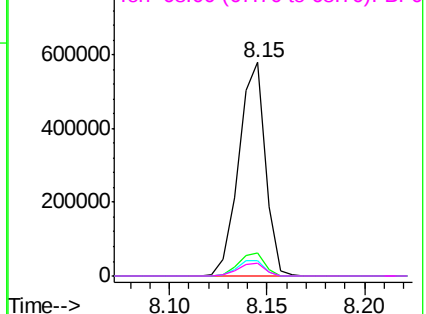


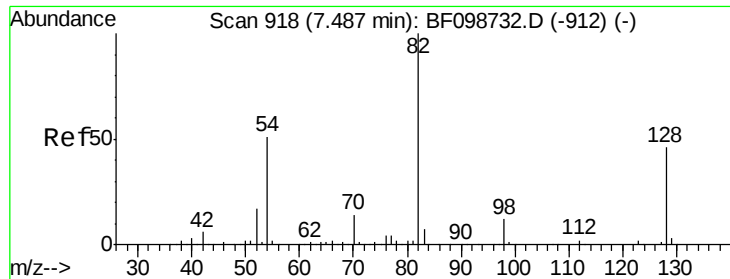




#23
 Nitrobenzene-d5
 Concen: 80.87 ng
 RT: 7.43 min Scan# 908
 Delta R.T. -0.01 min
 Lab File: BF099153.D
 Acq: 6 Oct 2017 17:56

Instrument :
 BNA_F
 ClientSampleId :
 PB102940BL

Tgt Ion: 82 Resp: 690764
 Ion Ratio Lower Upper
 82 100
 128 47.4 36.1 54.1
 54 47.6 41.4 62.2

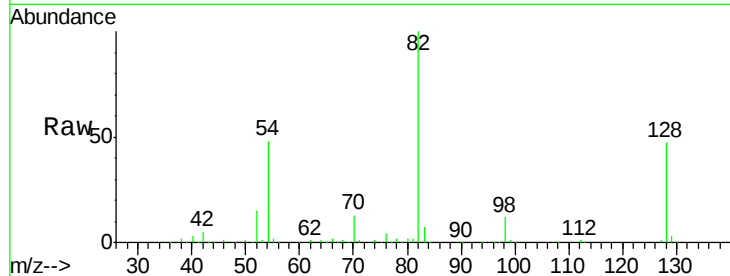


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

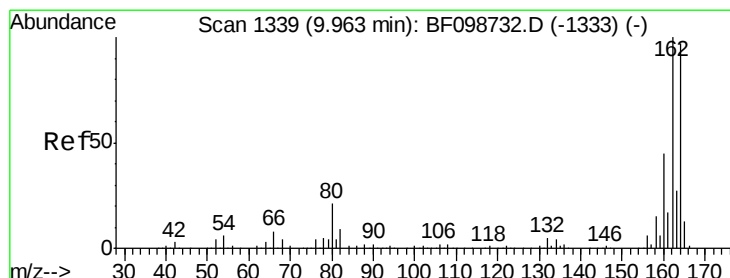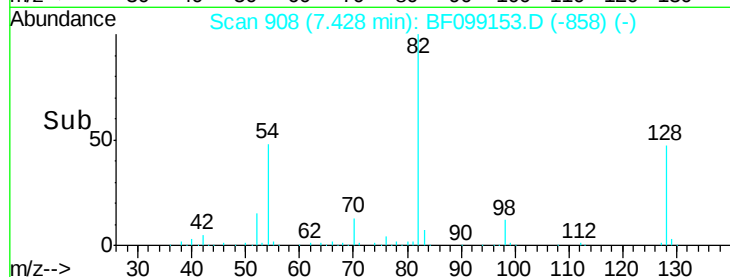
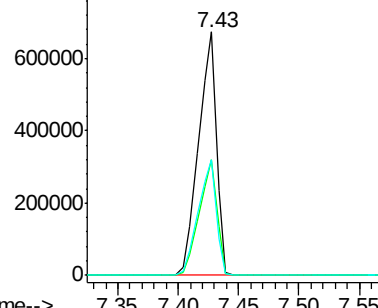



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.90 min Scan# 1328
 Delta R.T. -0.01 min
 Lab File: BF099153.D
 Acq: 6 Oct 2017 17:56

Tgt Ion: 164 Resp: 249629
 Ion Ratio Lower Upper
 164 100
 162 103.2 86.1 129.1
 160 45.8 38.3 57.5

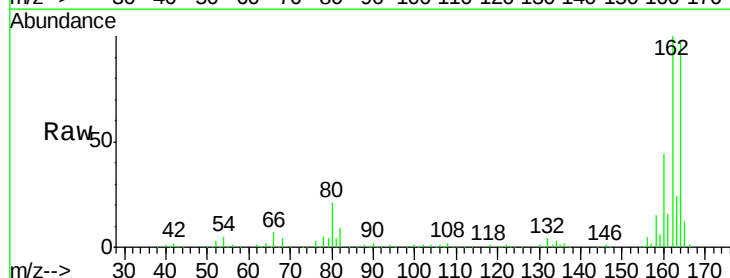

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E



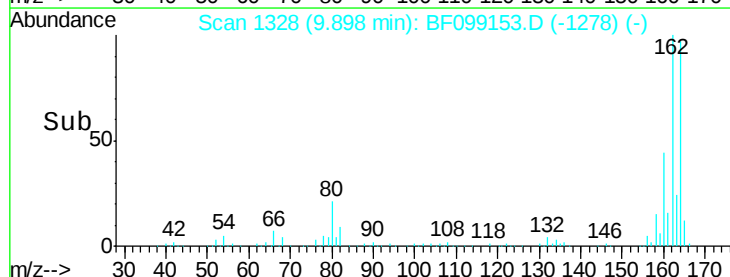
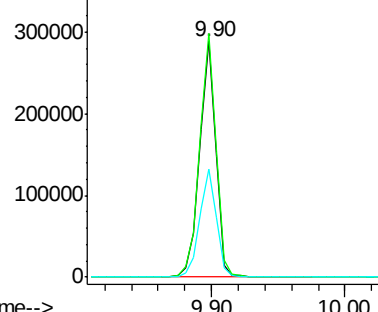


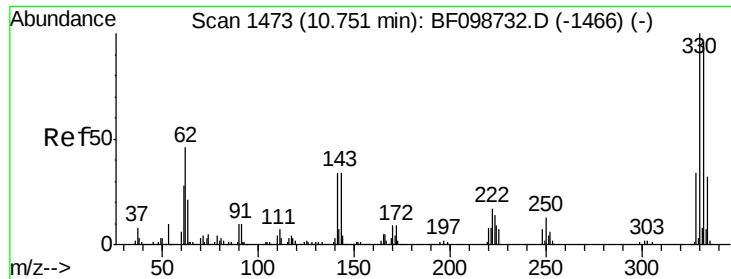

#41
 2,4,6-Tribromophenol
 Concen: 114.45 ng
 RT: 10.69 min Scan# 1463
 Delta R.T. -0.01 min
 Lab File: BF099153.D
 Acq: 6 Oct 2017 17:56




Instrument :
 BNA_F
 ClientSampleId :
 PB102940BL


Tgt Ion:330 Resp: 233787
 Ion Ratio Lower Upper
 330 100
 332 95.5 77.0 115.6
 141 38.2 29.9 44.9

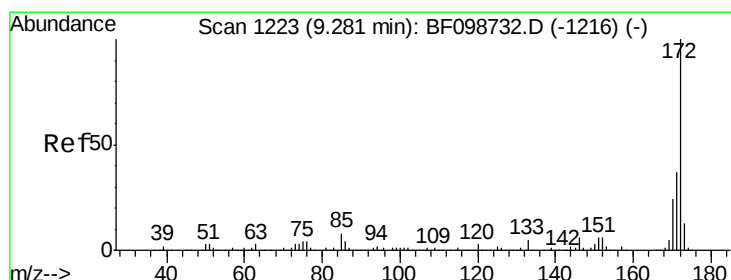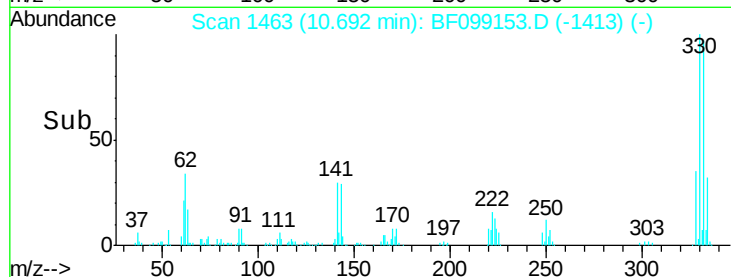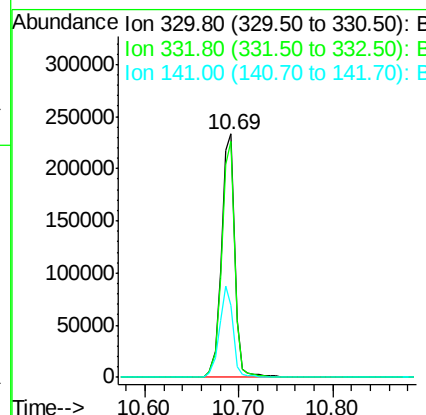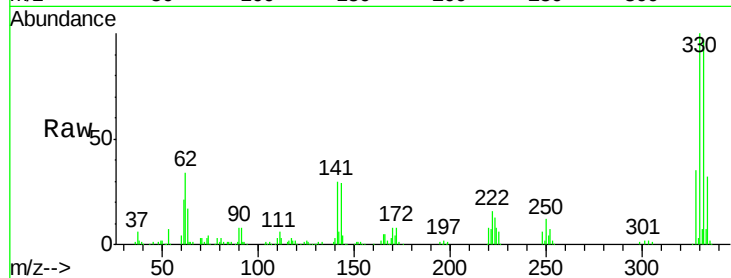

#44
 2-Fluorobiphenyl
 Concen: 84.34 ng
 RT: 9.22 min Scan# 1213
 Delta R.T. -0.01 min
 Lab File: BF099153.D
 Acq: 6 Oct 2017 17:56

Tgt Ion:172 Resp: 1261091
 Ion Ratio Lower Upper
 172 100
 171 35.7 29.7 44.5
 170 23.9 19.6 29.4

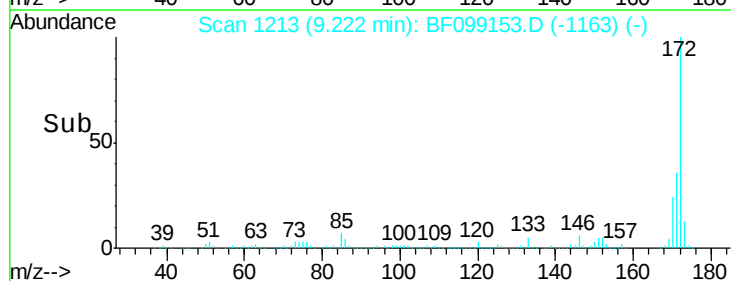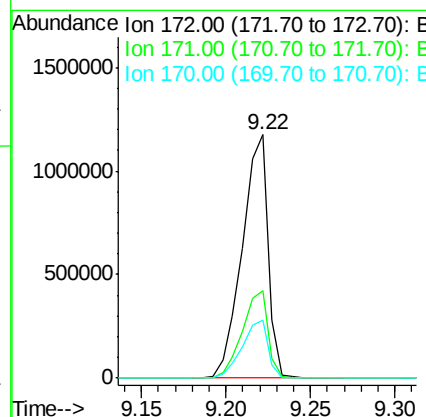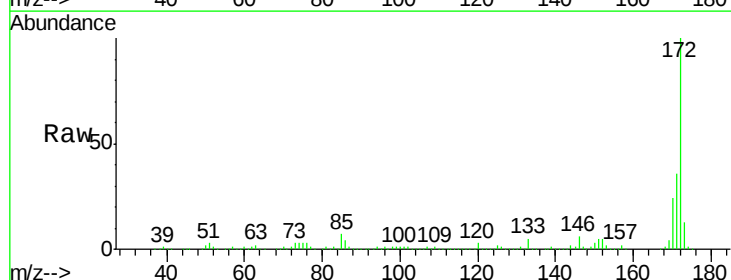


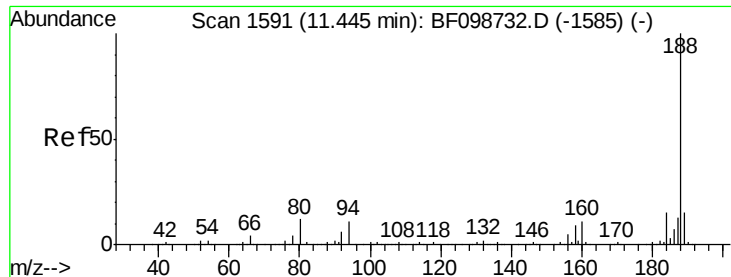




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.39 min Scan# 1581
Delta R.T. -0.01 min
Lab File: BF099153.D
Acq: 6 Oct 2017 17:56

Instrument :
BNA_F
ClientSampleId :
PB102940BL

Tgt Ion:188 Resp: 432602
Ion Ratio Lower Upper
188 100
94 10.5 8.5 12.7
80 11.0 9.2 13.8

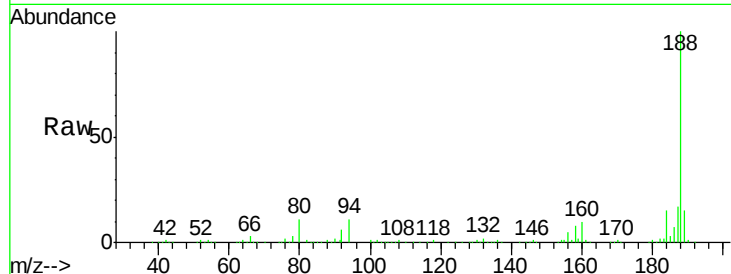


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

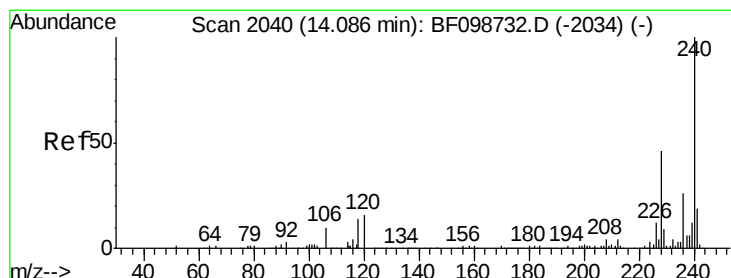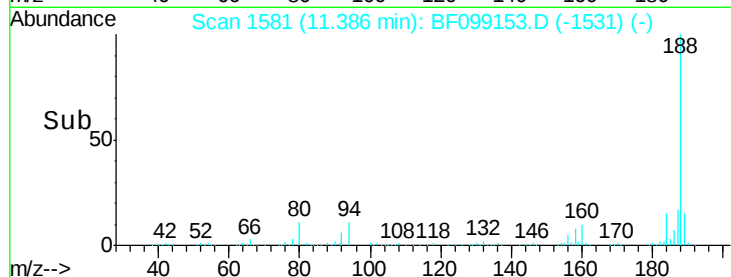
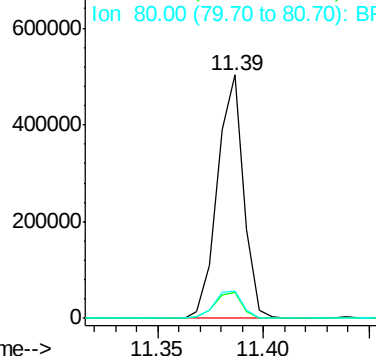



#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.02 min Scan# 2029
Delta R.T. -0.01 min
Lab File: BF099153.D
Acq: 6 Oct 2017 17:56

Tgt Ion:240 Resp: 301243
Ion Ratio Lower Upper
240 100
120 15.4 9.5 14.3#
236 25.9 20.7 31.1

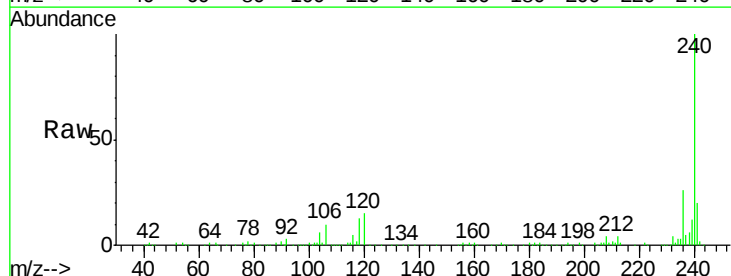

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

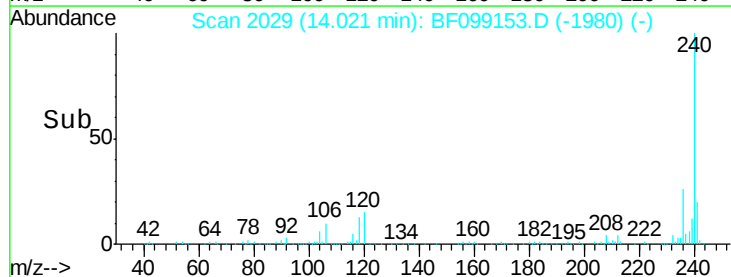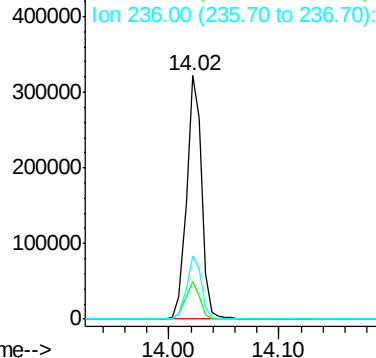

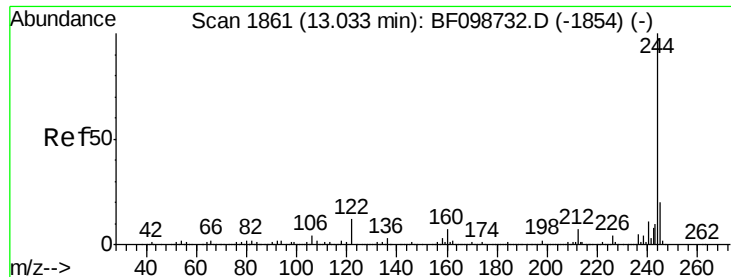

#78

Terphenyl-d14

Concen: 81.10 ng

RT: 12.97 min Scan# 1851

Delta R.T. -0.00 min

Lab File: BF099153.D

Acq: 6 Oct 2017 17:56

Instrument :

BNA_F

ClientSampleId :

PB102940BL


Tgt Ion:244 Resp: 1074282

Ion Ratio Lower Upper

244 100

212 7.2 5.4 8.0




122 12.5 11.0 16.4

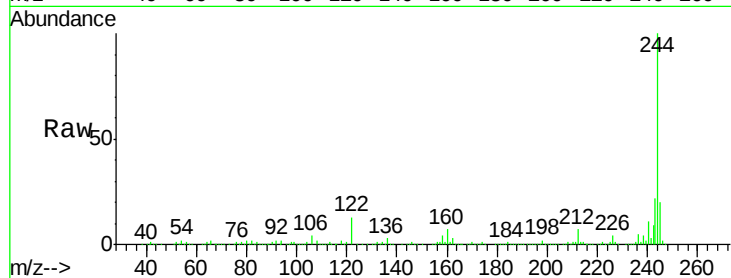

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

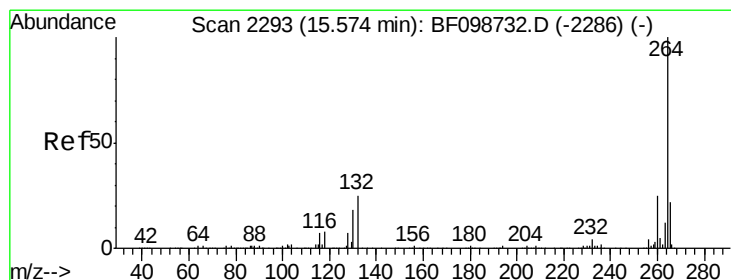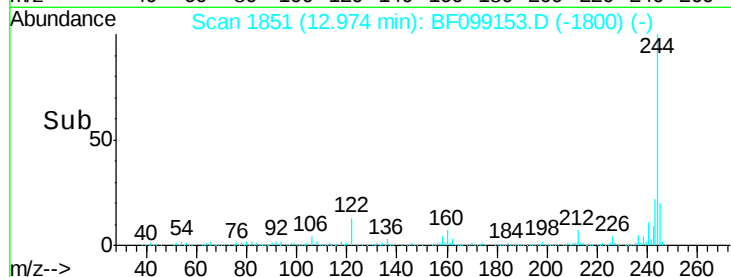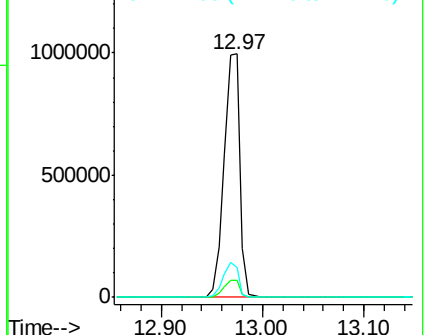

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.50 min Scan# 2280

Delta R.T. -0.01 min

Lab File: BF099153.D

Acq: 6 Oct 2017 17:56


Tgt Ion:264 Resp: 228209

Ion Ratio Lower Upper

264 100

260 23.7 19.2 28.8

265 21.5 17.5 26.3

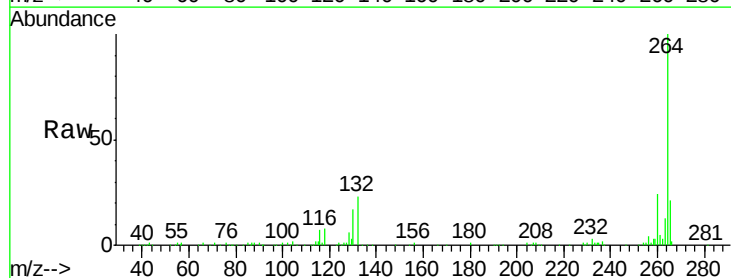

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

