

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100617\
 Data File : BF099158.D
 Acq On : 6 Oct 2017 20:15
 Operator : SJ/JU
 Sample : I5571-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PAMT-COMP-C-D

Quant Time: Oct 06 23:50:47 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 05 17:20:48 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	146763	20.00	ng	0.00
21) Naphthalene-d8	8.15	136	605858	20.00	ng	0.00
38) Acenaphthene-d10	9.90	164	274383	20.00	ng	0.00
63) Phenanthrene-d10	11.39	188	490984	20.00	ng	0.00
75) Chrysene-d12	14.02	240	344777	20.00	ng	-0.01
86) Perylene-d12	15.50	264	249093	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	191107	20.73	ng	0.00
7) Phenol-d6	6.48	99	147359	12.96	ng	-0.02
23) Nitrobenzene-d5	7.42	82	398962	42.23	ng	-0.01
41) 2,4,6-Tribromophenol	10.69	330	99035	44.11	ng	-0.01
44) 2-Fluorobiphenyl	9.22	172	748821	45.56	ng	-0.01
78) Terphenyl-d14	12.97	244	685798	45.24	ng	0.00
Target Compounds						
10) Phenol	6.50	94	28618	2.25	ng	97
49) Dimethylphthalate	9.61	163	176054	8.50	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100617\
Data File : BF099158.D
Acq On : 6 Oct 2017 20:15
Operator : SJ/JU
Sample : I5571-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PAMT-COMP-C-D

Quant Time: Oct 06 23:50:47 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 05 17:20:48 2017
Response via : Initial Calibration

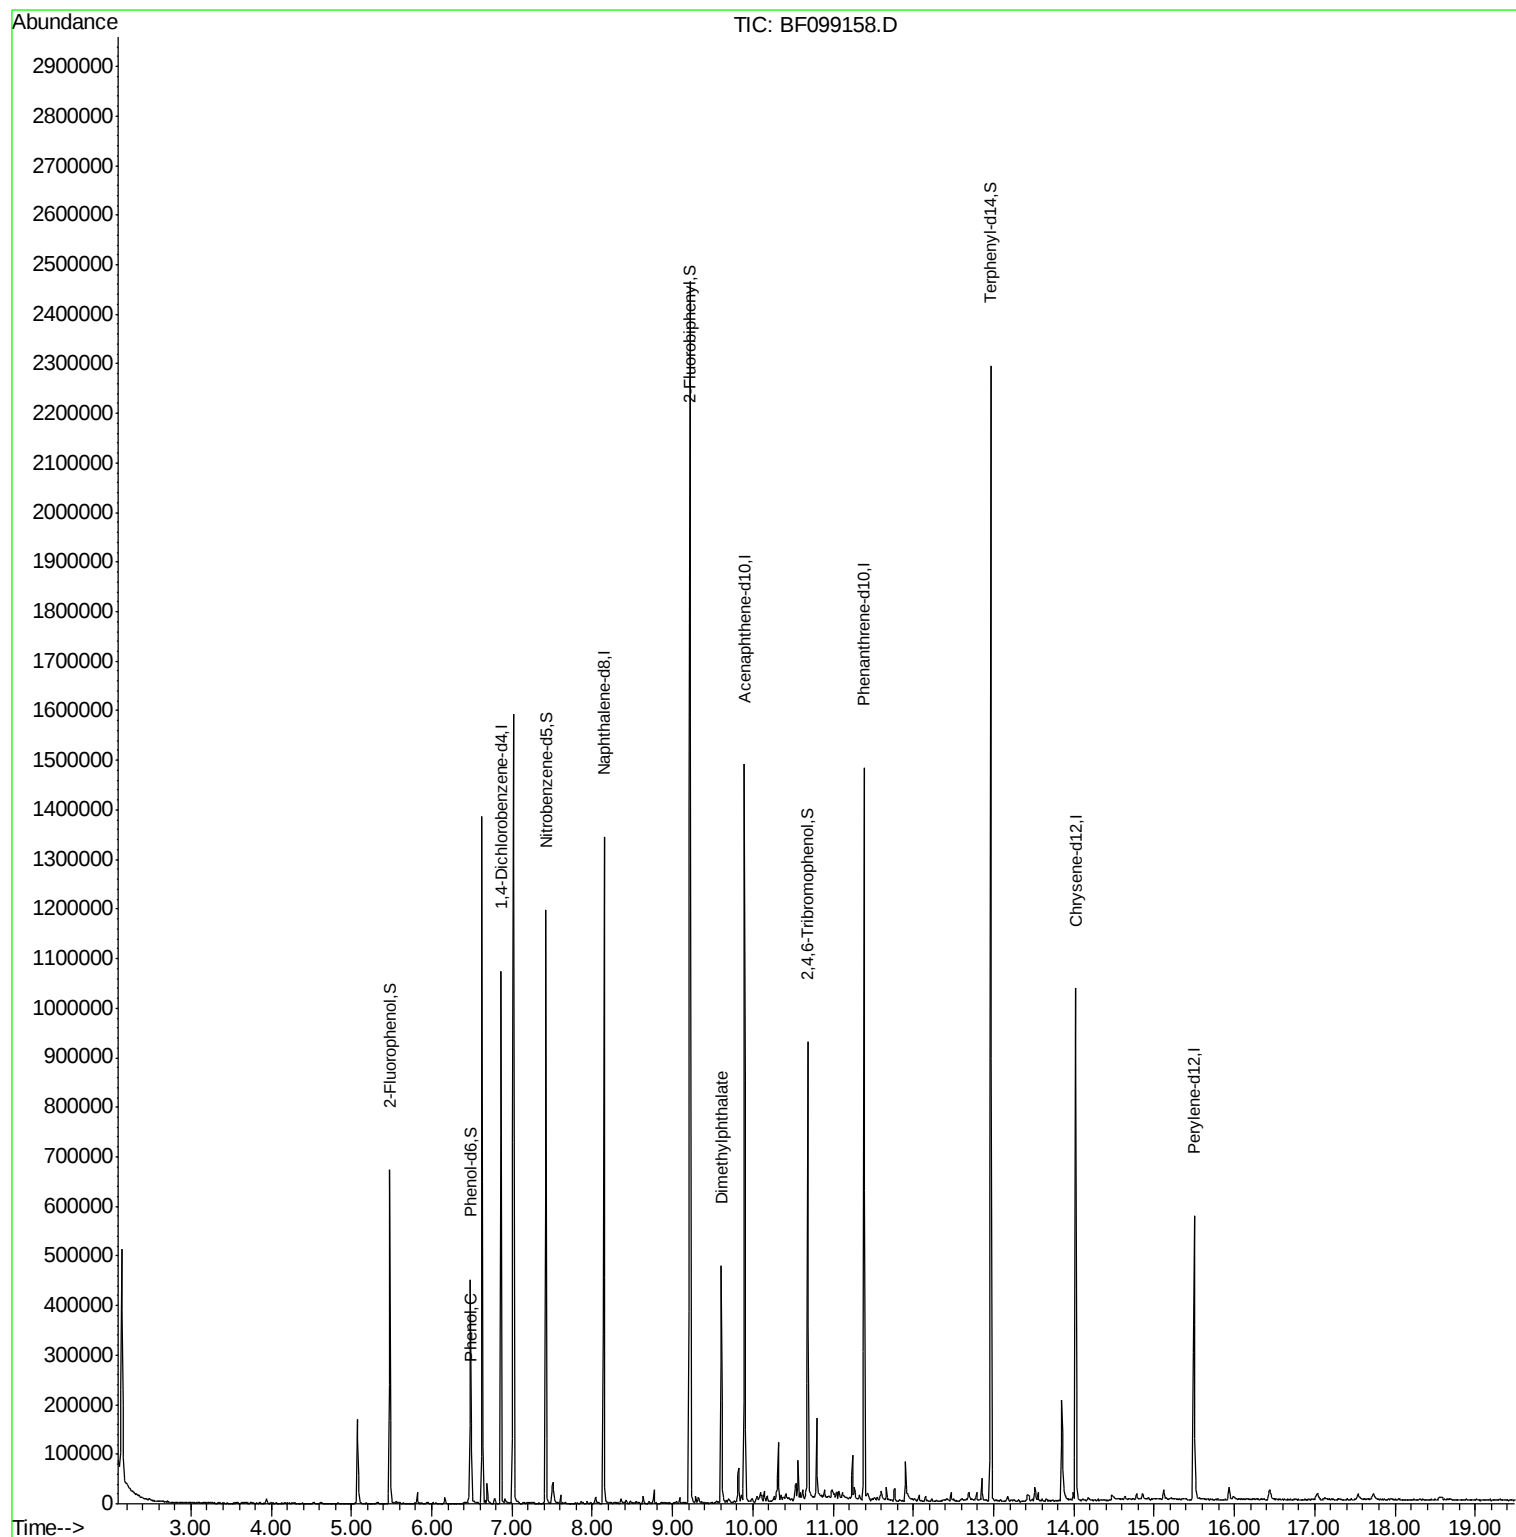

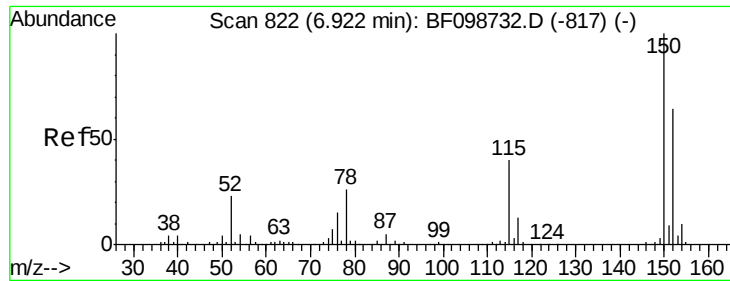


#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.86 min Scan# 812
 Delta R.T. -0.01 min
 Lab File: BF099158.D
 Acq: 6 Oct 2017 20:15

Instrument :
 BNA_F
 ClientSampleId :
 PAMT-COMP-C-D

Tgt Ion:152 Resp: 146763
 Ion Ratio Lower Upper
 152 100
 150 156.5 124.6 186.8
 115 60.8 50.1 75.1

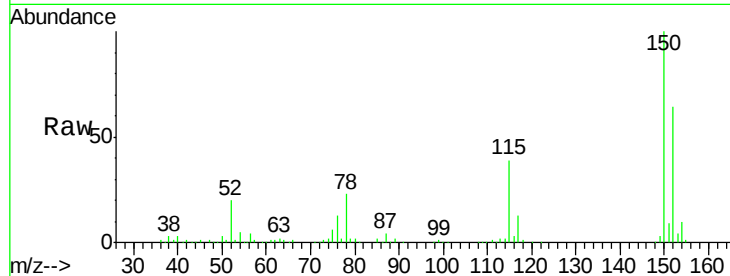


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

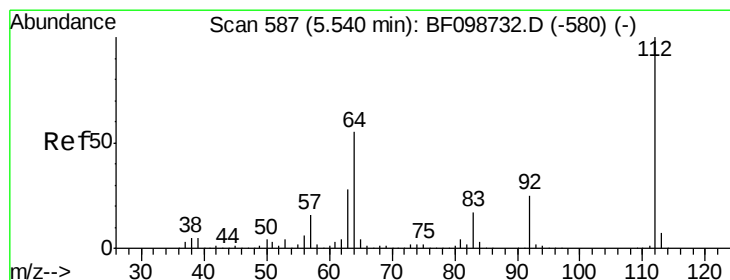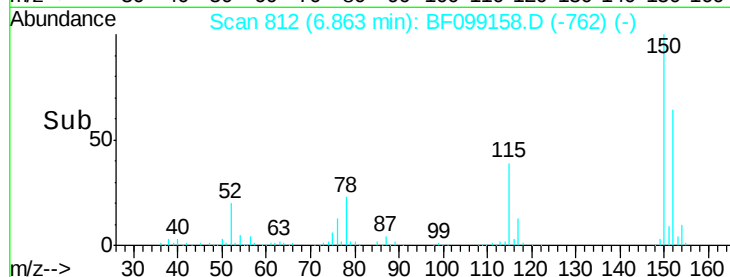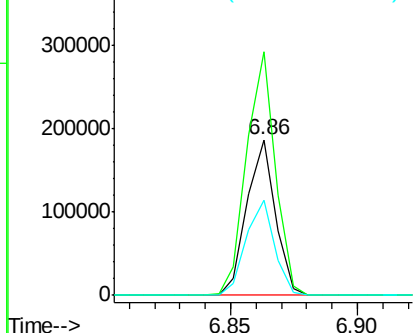



#5


2-Fluorophenol
 Concen: 20.73 ng
 RT: 5.47 min Scan# 576
 Delta R.T. -0.01 min
 Lab File: BF099158.D
 Acq: 6 Oct 2017 20:15

Tgt Ion:112 Resp: 191107
 Ion Ratio Lower Upper
 112 100
 64 58.0 47.9 71.9
 63 29.0 23.7 35.5

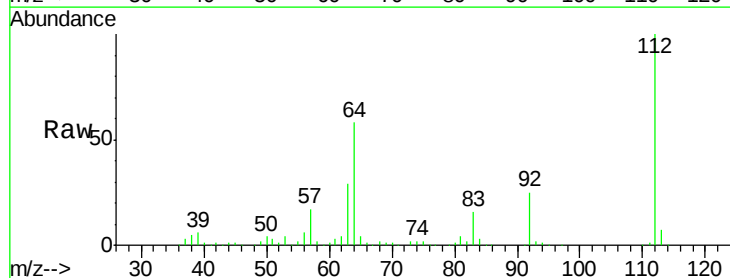

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

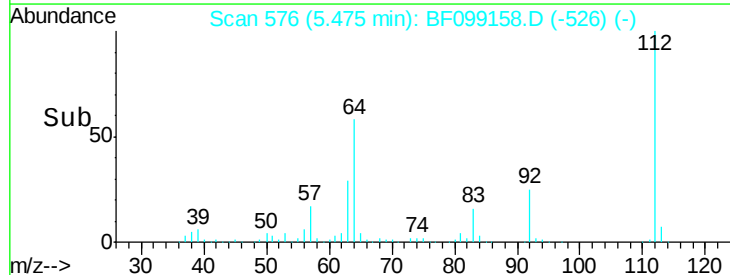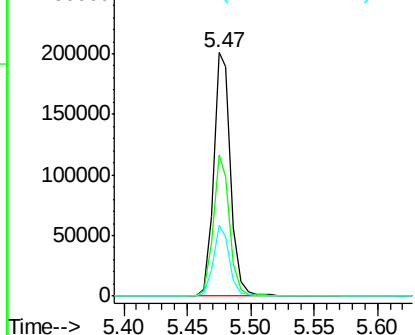

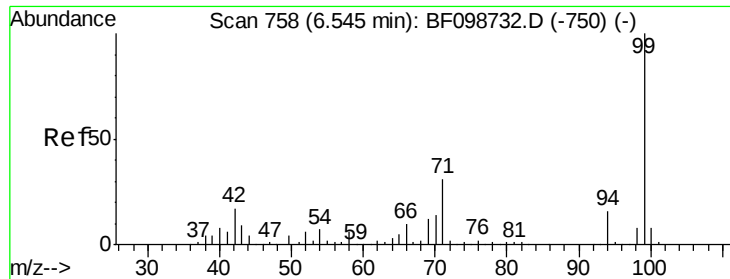

#7

Phenol-d6

Concen: 12.96 ng

RT: 6.48 min Scan# 747

Delta R.T. -0.02 min

Lab File: BF099158.D

Acq: 6 Oct 2017 20:15

Instrument :

BNA_F

ClientSampleId :

PAMT-COMP-C-D


Tgt Ion: 99 Resp: 147359

Ion Ratio Lower Upper

99 100

42 16.9 14.5 21.7




71 31.1 25.4 38.0

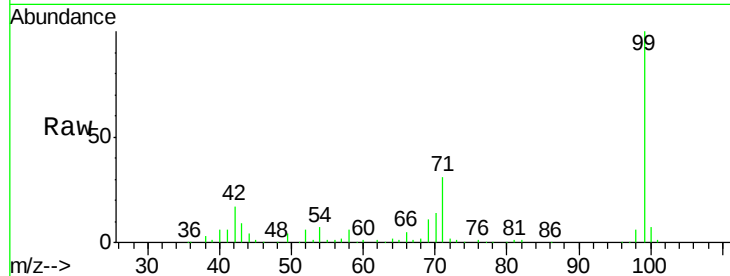

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

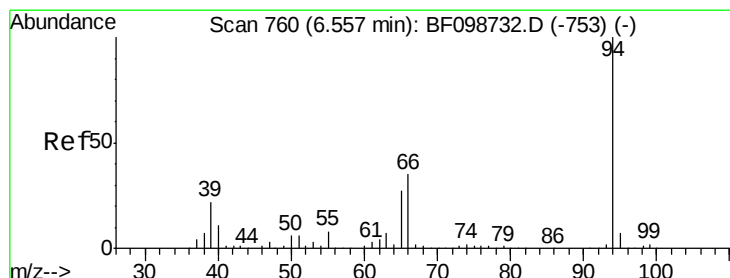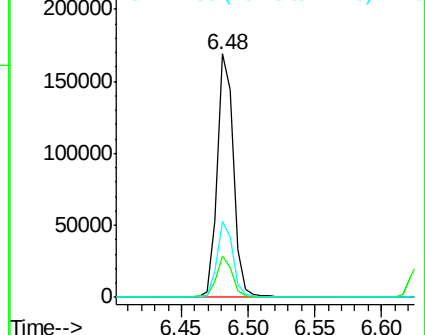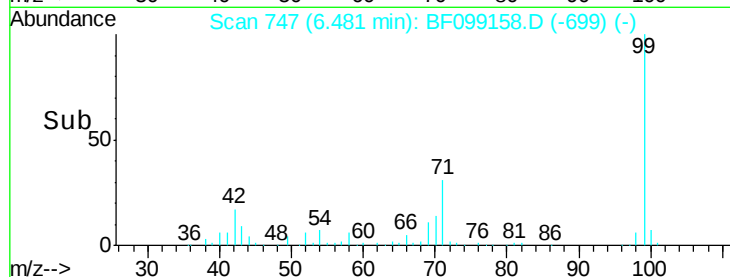

#10

Phenol

Concen: 2.25 ng

RT: 6.50 min Scan# 750

Delta R.T. -0.02 min

Lab File: BF099158.D

Acq: 6 Oct 2017 20:15


Tgt Ion: 94 Resp: 28618

Ion Ratio Lower Upper

94 100

65 25.3 7.9 47.9



66 35.0 16.2 56.2

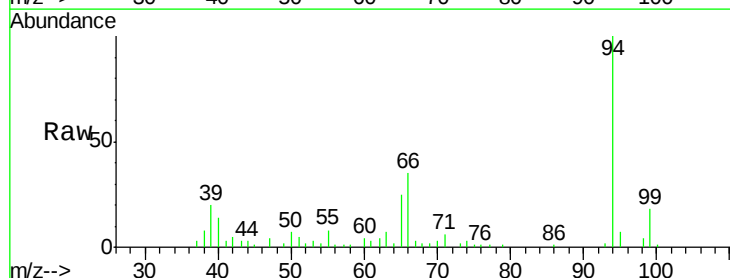


Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

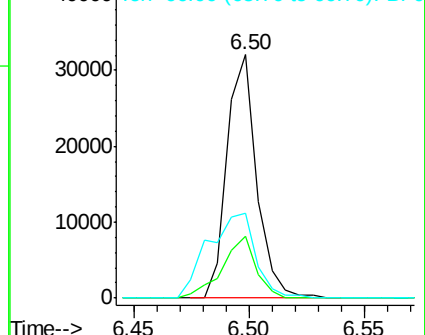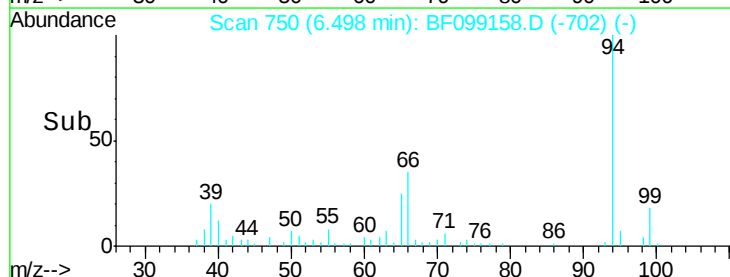


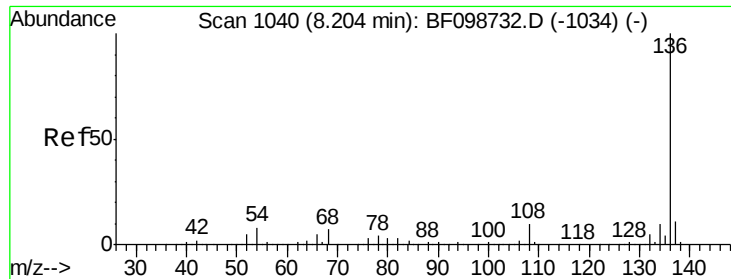




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.15 min Scan# 1030
Delta R.T. -0.01 min
Lab File: BF099158.D
Acq: 6 Oct 2017 20:15

Instrument :
BNA_F
ClientSampleId :
PAMT-COMP-C-D

Tgt Ion: 136 Resp: 605858
Ion Ratio Lower Upper
136 100
137 10.9 8.9 13.3
54 7.2 6.6 9.8
68 5.8 5.0 7.4

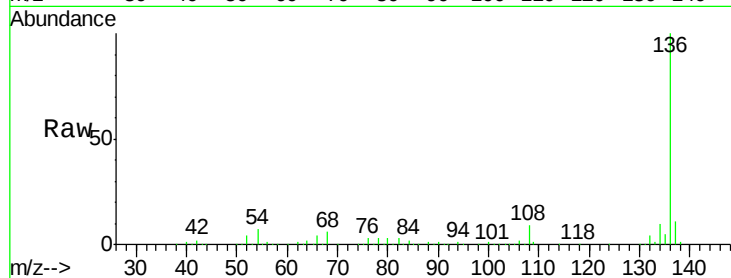


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

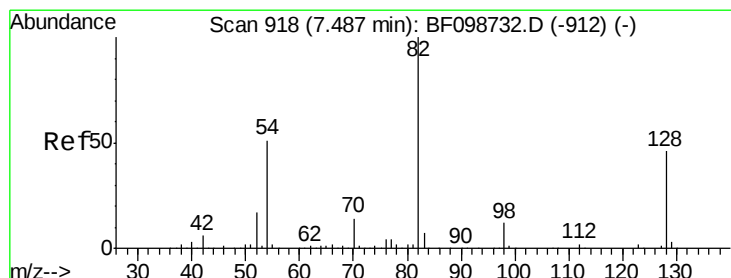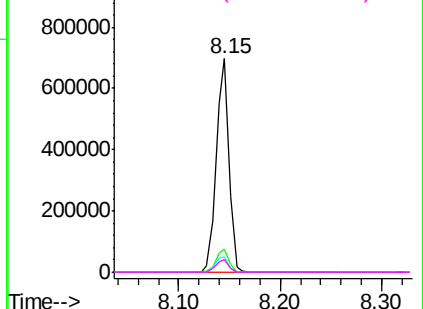
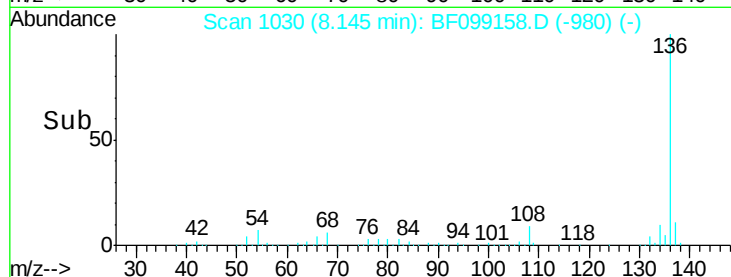



#23
Nitrobenzene-d5
Concen: 42.23 ng
RT: 7.42 min Scan# 907
Delta R.T. -0.01 min
Lab File: BF099158.D
Acq: 6 Oct 2017 20:15

Tgt Ion: 82 Resp: 398962
Ion Ratio Lower Upper
82 100
128 45.6 36.1 54.1
54 50.2 41.4 62.2

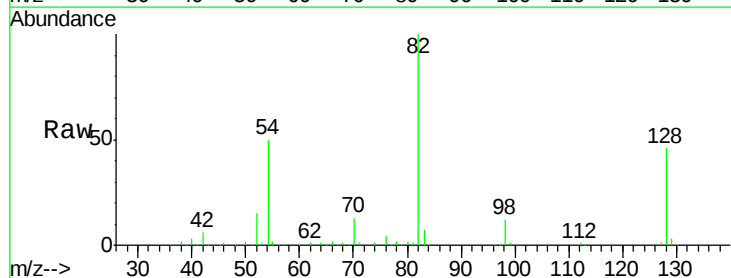

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

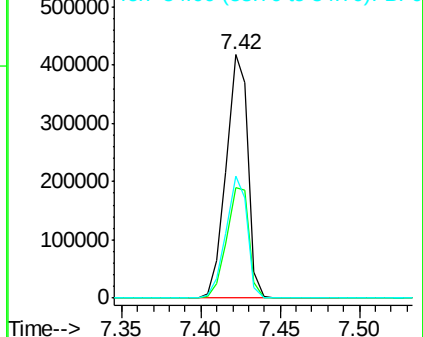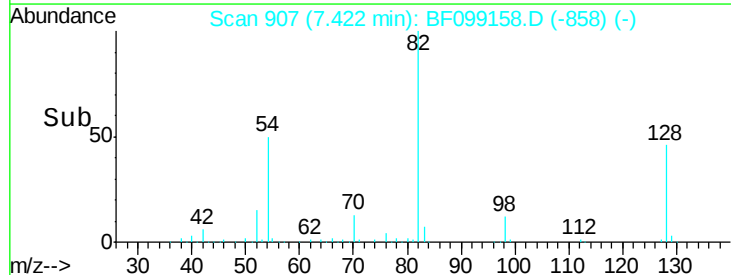


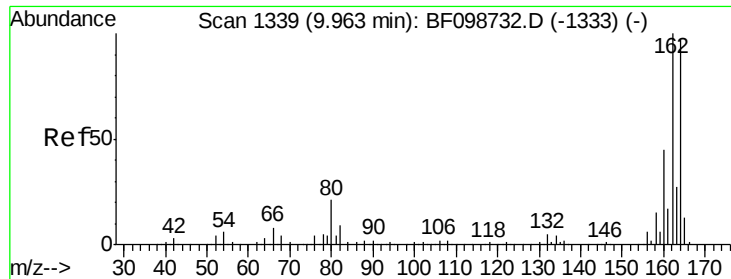




#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.90 min Scan# 1328
 Delta R.T. -0.01 min
 Lab File: BF099158.D
 Acq: 6 Oct 2017 20:15

Instrument :
 BNA_F
 ClientSampleId :
 PAMT-COMP-C-D

Tgt Ion:164 Resp: 274383
 Ion Ratio Lower Upper
 164 100
 162 103.7 86.1 129.1
 160 45.9 38.3 57.5

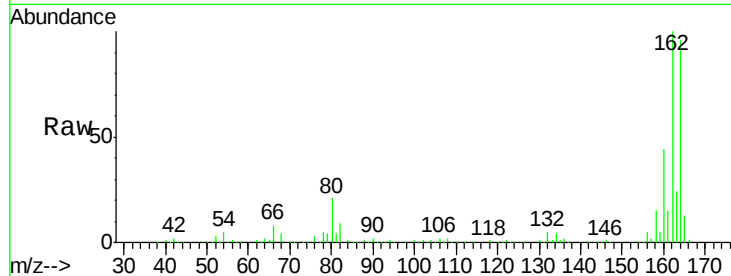


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

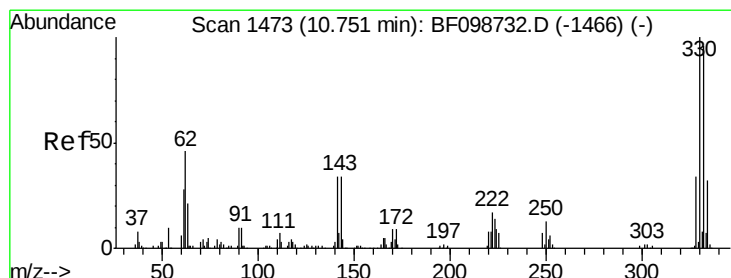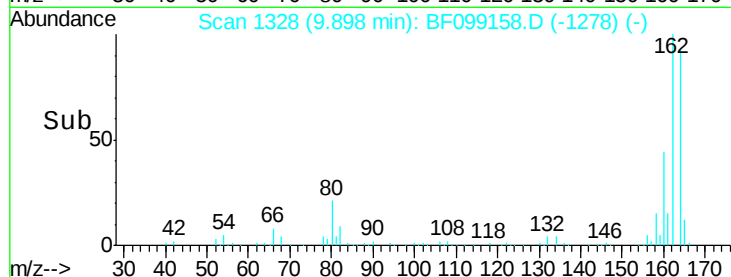
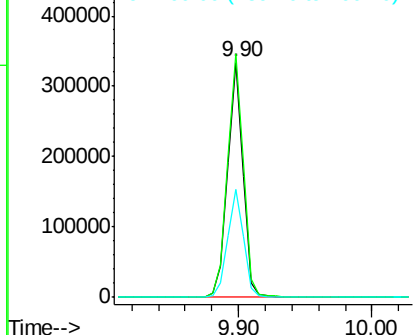



#41
 2,4,6-Tribromophenol
 Concen: 44.11 ng
 RT: 10.69 min Scan# 1462
 Delta R.T. -0.01 min
 Lab File: BF099158.D
 Acq: 6 Oct 2017 20:15

Tgt Ion:330 Resp: 99035
 Ion Ratio Lower Upper
 330 100
 332 95.2 77.0 115.6
 141 41.6 29.9 44.9

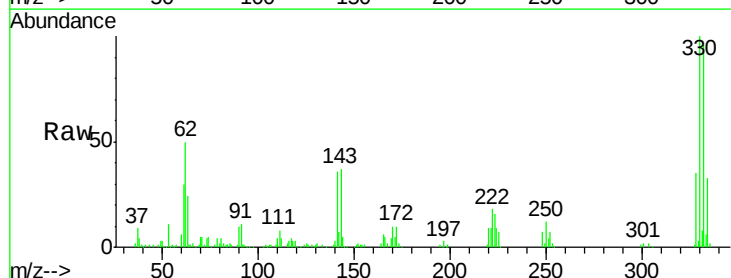

Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E



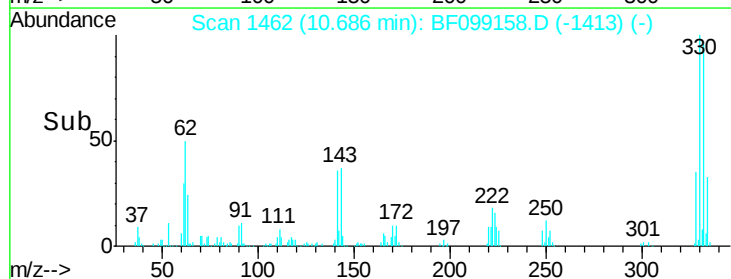
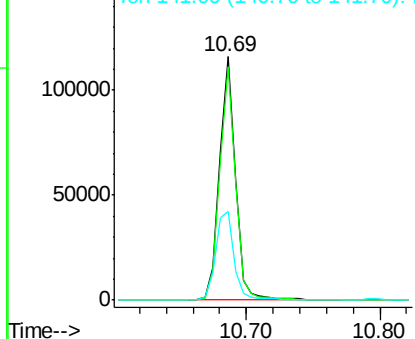


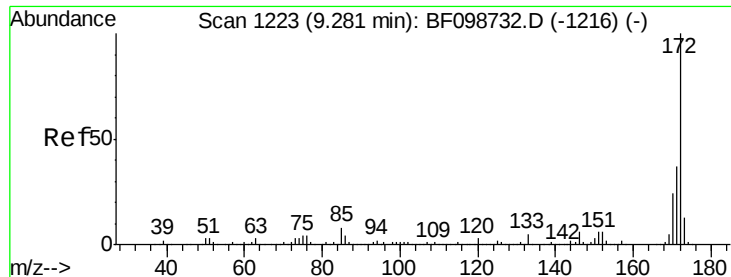

#44
 2-Fluorobiphenyl
 Concen: 45.56 ng
 RT: 9.22 min Scan# 1212
 Delta R.T. -0.01 min
 Lab File: BF099158.D
 Acq: 6 Oct 2017 20:15




Instrument :
 BNA_F
 ClientSampleId :
 PAMT-COMP-C-D


Tgt Ion:172 Resp: 748821
 Ion Ratio Lower Upper
 172 100
 171 36.6 29.7 44.5
 170 23.5 19.6 29.4

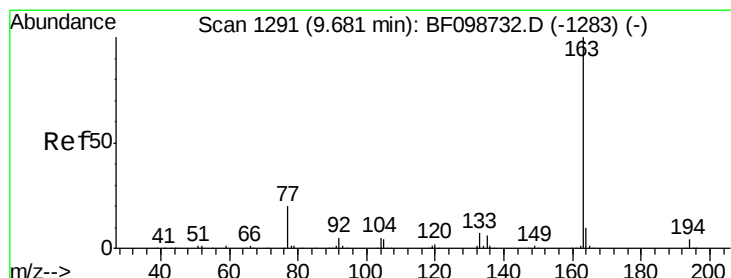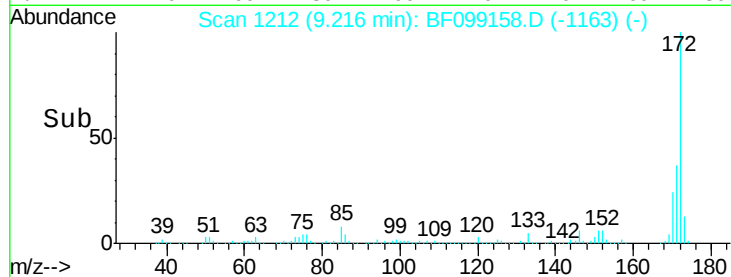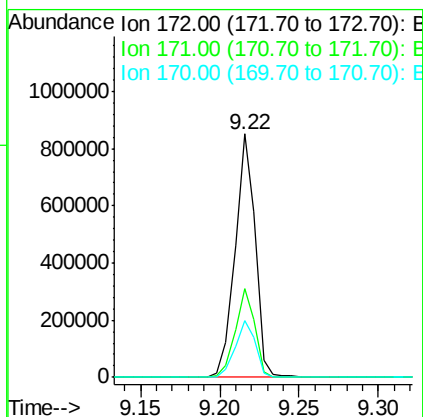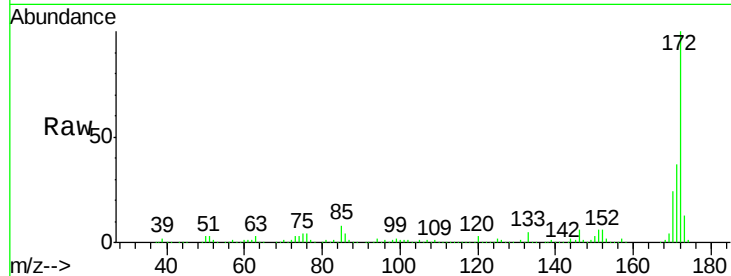

#49
 Dimethylphthalate
 Concen: 8.50 ng
 RT: 9.61 min Scan# 1279
 Delta R.T. -0.02 min
 Lab File: BF099158.D
 Acq: 6 Oct 2017 20:15

Tgt Ion:163 Resp: 176054
 Ion Ratio Lower Upper
 163 100
 194 3.3 2.7 4.1
 164 10.4 8.2 12.2

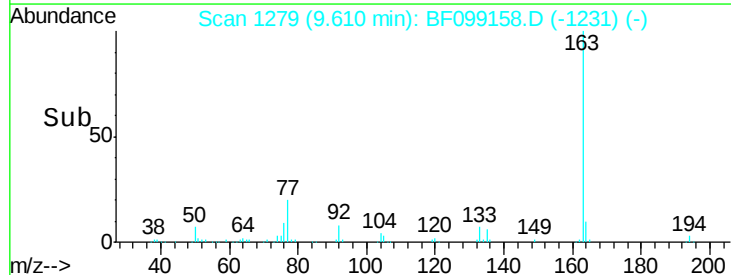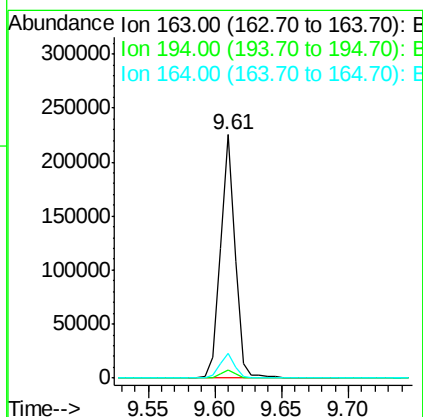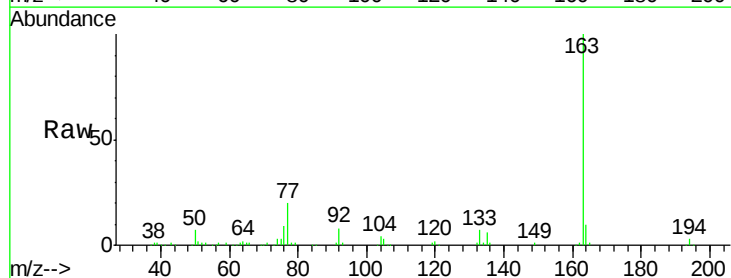


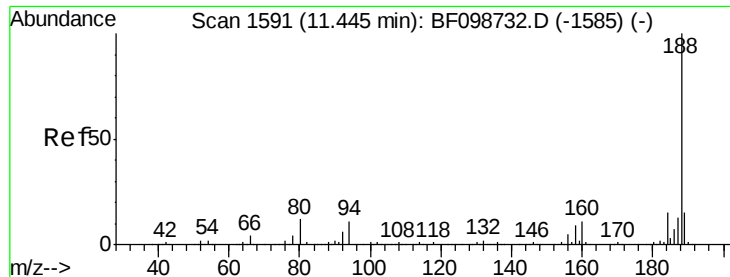




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.39 min Scan# 1581
Delta R.T. -0.01 min
Lab File: BF099158.D
Acq: 6 Oct 2017 20:15

Instrument :
BNA_F
ClientSampleId :
PAMT-COMP-C-D

Tgt Ion:188 Resp: 490984
Ion Ratio Lower Upper
188 100
94 10.4 8.5 12.7
80 11.5 9.2 13.8

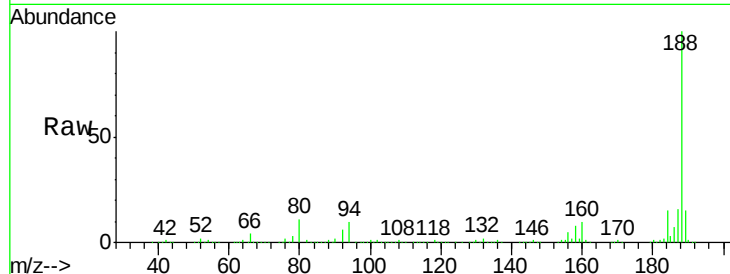


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

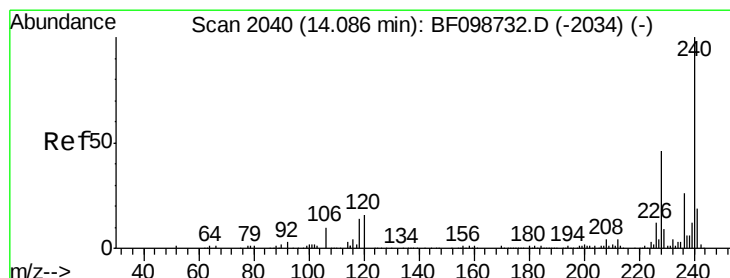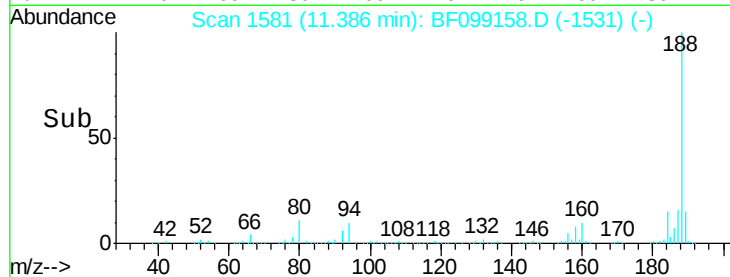
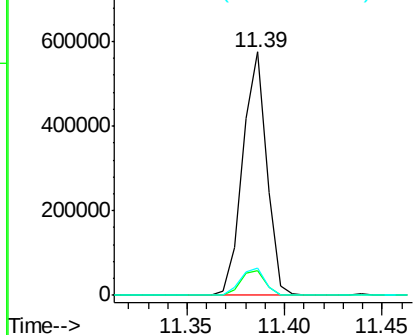



#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.02 min Scan# 2029
Delta R.T. -0.01 min
Lab File: BF099158.D
Acq: 6 Oct 2017 20:15

Tgt Ion:240 Resp: 344777
Ion Ratio Lower Upper
240 100
120 15.5 9.5 14.3#
236 26.3 20.7 31.1

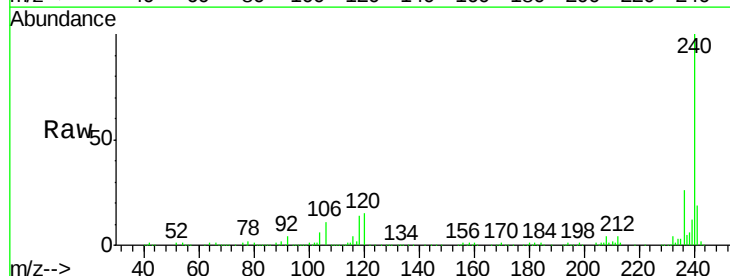

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



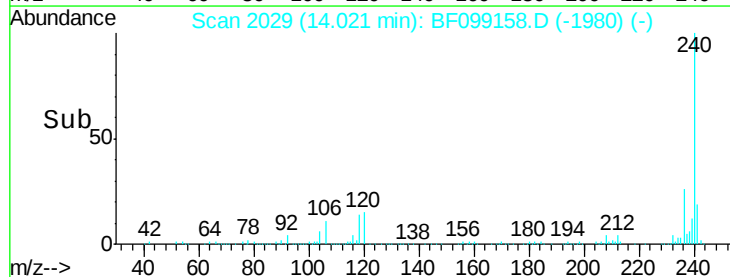
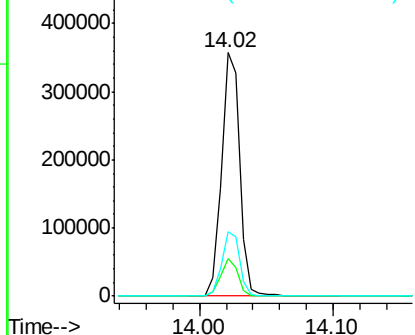


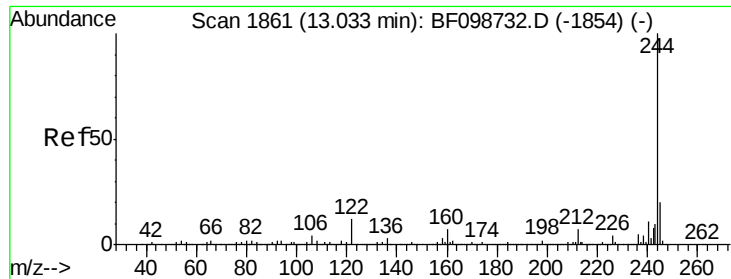

#78
 Terphenyl-d14
 Concen: 45.24 ng
 RT: 12.97 min Scan# 1850
 Delta R.T. -0.01 min
 Lab File: BF099158.D
 Acq: 6 Oct 2017 20:15

Instrument :
 BNA_F
 ClientSampleId :
 PAMT-COMP-C-D

Tgt Ion:244 Resp: 685798
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.4 8.0
 122 13.3 11.0 16.4

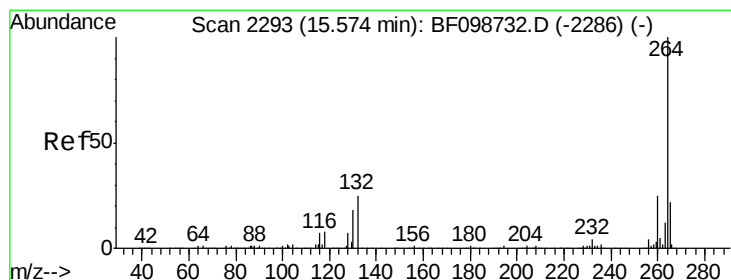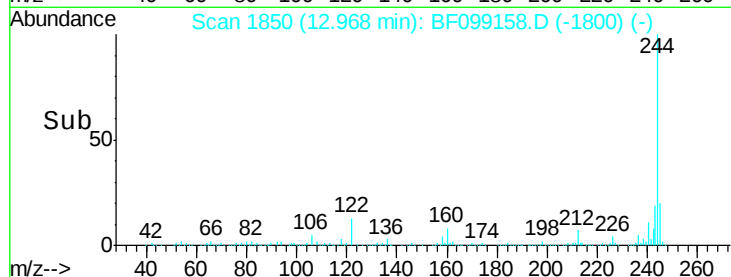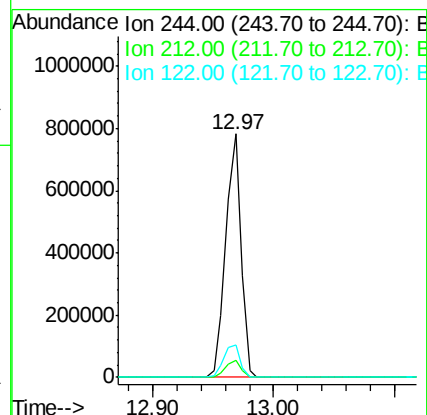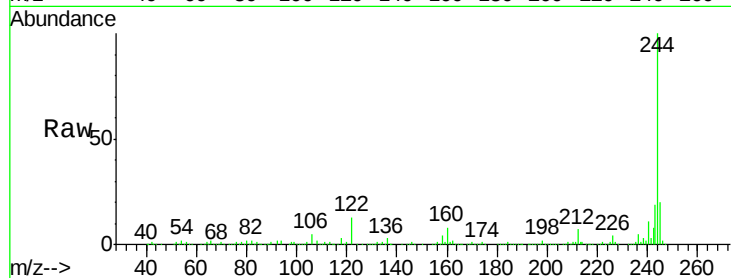

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.50 min Scan# 2280
 Delta R.T. -0.01 min
 Lab File: BF099158.D
 Acq: 6 Oct 2017 20:15

Tgt Ion:264 Resp: 249093
 Ion Ratio Lower Upper
 264 100
 260 24.1 19.2 28.8
 265 20.9 17.5 26.3

