


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF100617\  
Data File : BF099173.D  
Acq On : 7 Oct 2017 3:43  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF092317.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Oct 05 17:20:48 2017

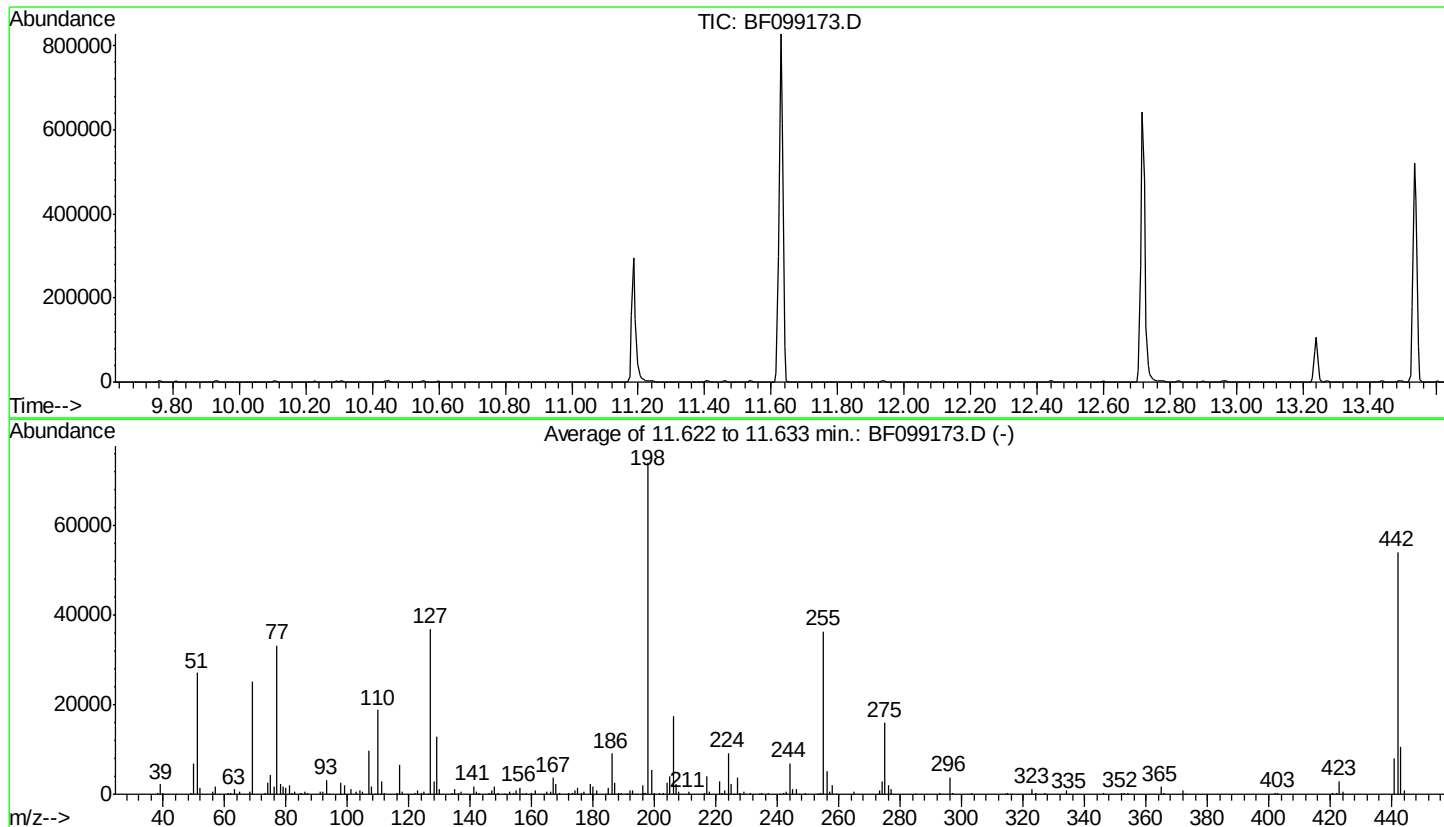

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1617

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 36.7      | 27144   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.8       | 452     | PASS             |
| 69          | 198          | 0.00         | 100          | 33.9      | 25069   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 49.9      | 36954   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.3       | 211     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 74032   | PASS             |
| 199         | 198          | 5            | 9            | 7.2       | 5299    | PASS             |
| 275         | 198          | 10           | 60           | 21.6      | 15974   | PASS             |
| 365         | 198          | 1            | 100          | 2.2       | 1657    | PASS             |
| 441         | 442          | 0.01         | 24           | 14.9      | 8069    | PASS             |
| 442         | 198          | 50           | 100          | 73.1      | 54119   | PASS             |
| 443         | 442          | 15           | 24           | 19.5      | 10554   | PASS             |