
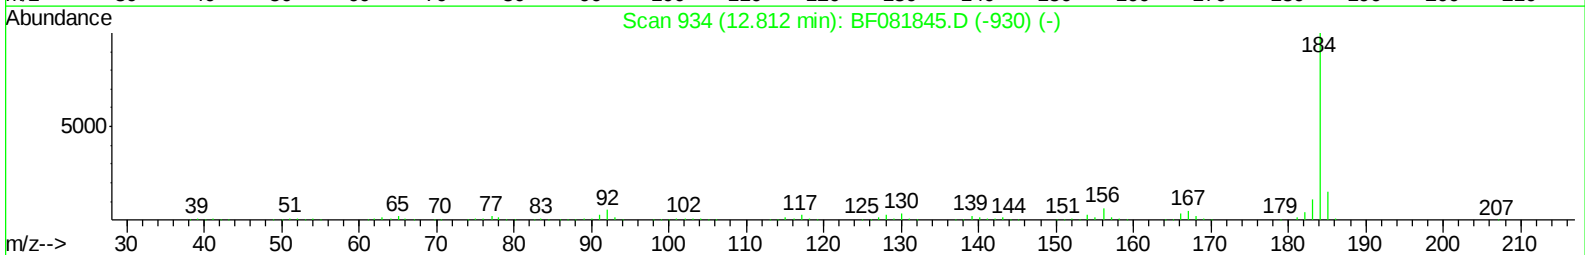
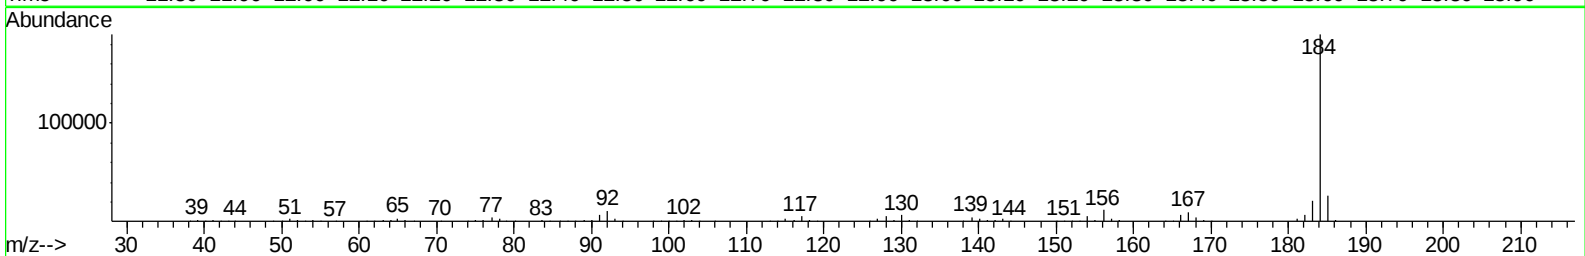


Data Path : Z:\HPCHEM1\BNA F\DATA\BF100715\
Data File : BF082100.D
Acq On : 7 Oct 2015 11:10
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 04:28:14 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 08 02:46:05 2015
Response via : Initial Calibration

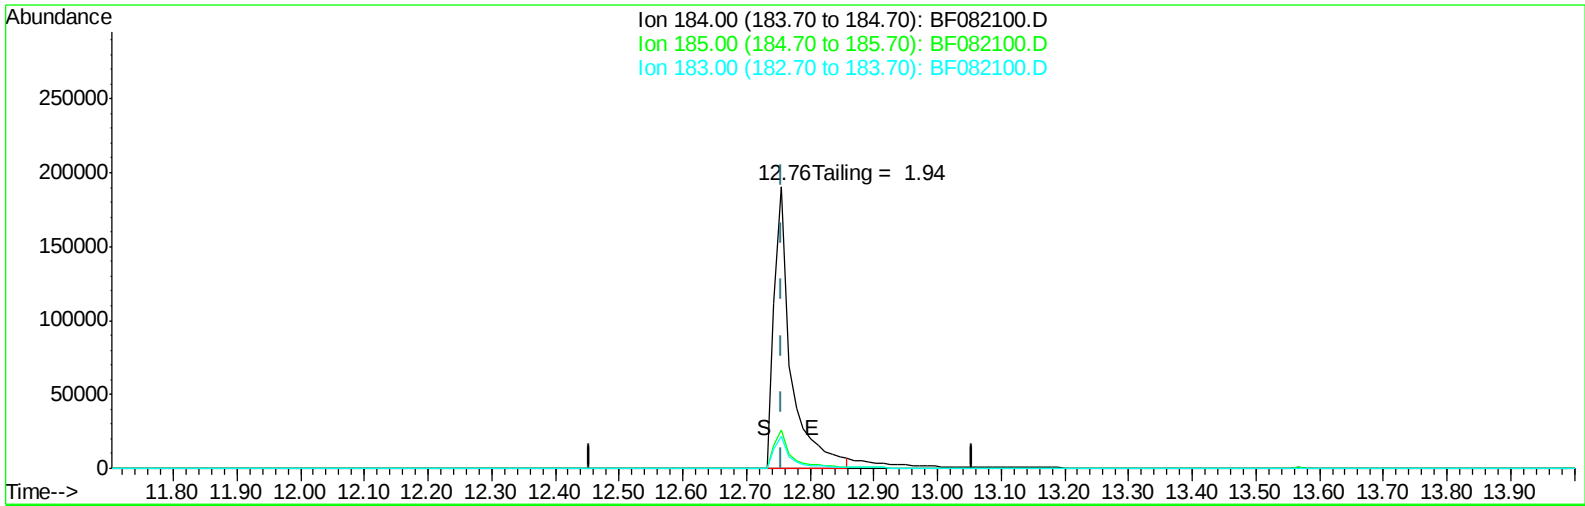

TIC: BF082100.D

(76) Benzidine




12.755min (-0.000) 0.00ng m

response 349330

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.86
183.00	9.50	11.19
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100715\
Data File : BF082100.D
Acq On : 7 Oct 2015 11:10
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 04:28:14 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 08 02:46:05 2015
Response via : Initial Calibration

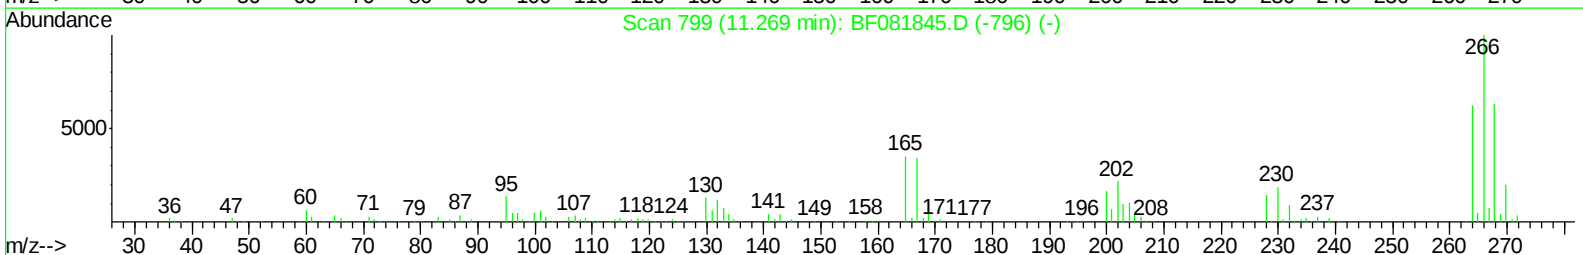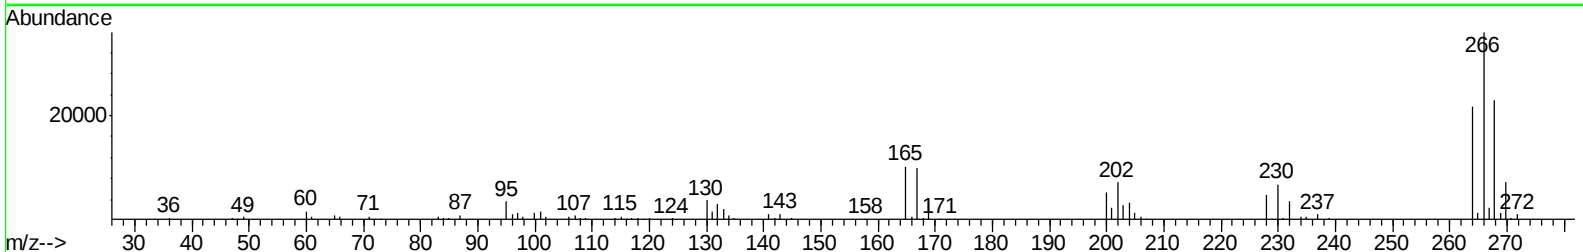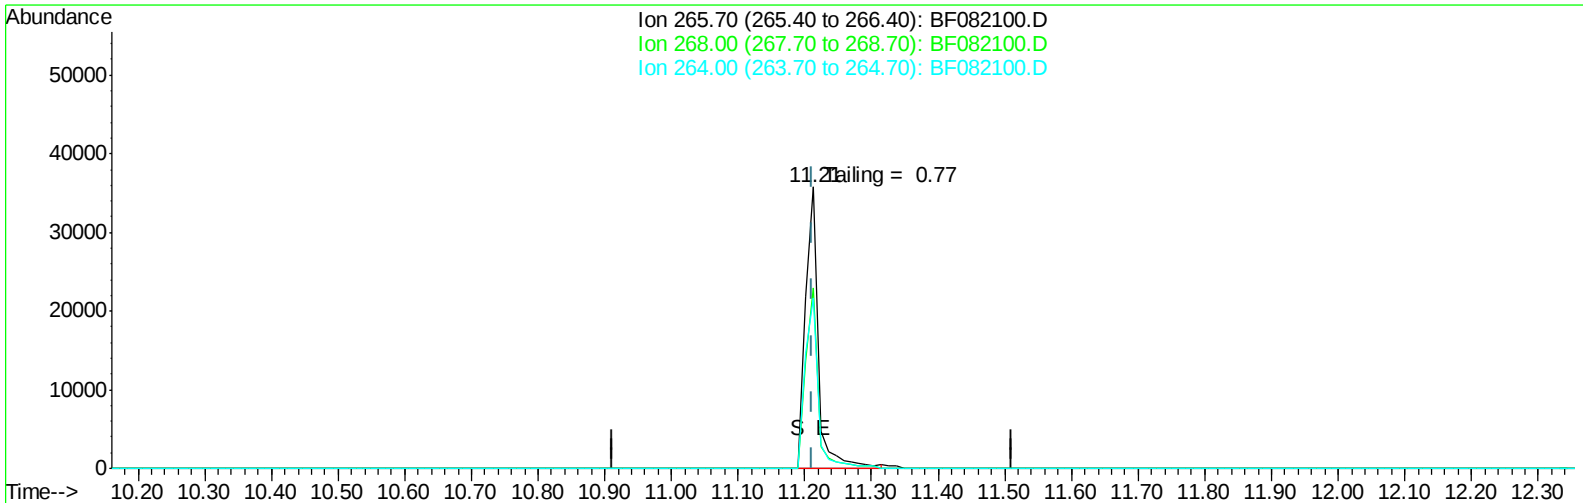

TIC: BF082100.D

(69) Pentachlorophenol (C)

11.212min (-0.000) 0.00ng

response 48200

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	64.04
264.00	62.70	60.60
0.00	0.00	0.00