


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100715\
 Data File : BF082100.D
 Acq On : 7 Oct 2015 11:10
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 08 02:46:05 2015

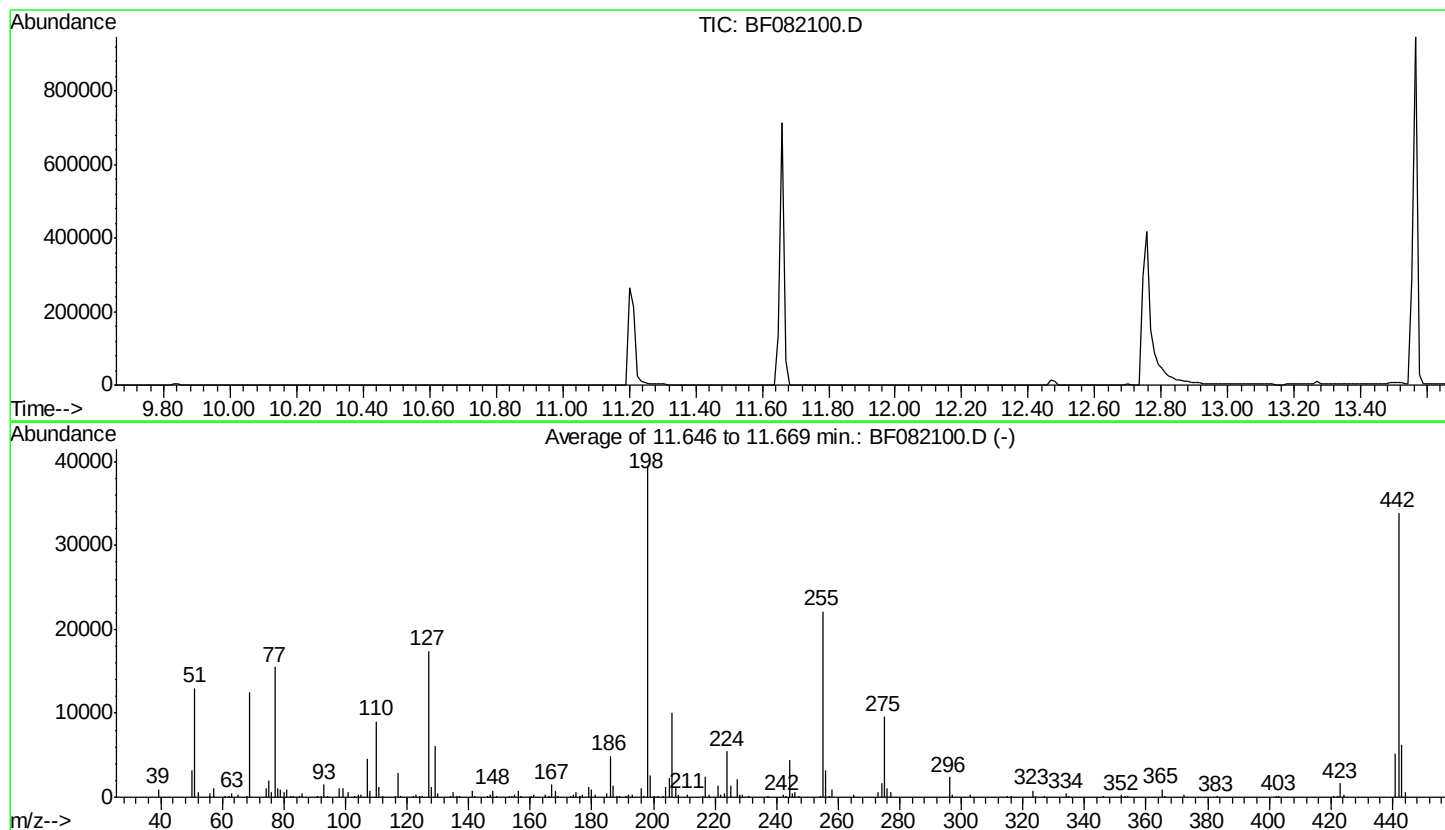

AutoFind: Scans 832, 833, 834; Background Corrected with Scan 829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	13034	PASS
68	69	0.00	2	0.9	116	PASS
69	198	0.00	100	31.6	12471	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.2	17465	PASS
197	198	0.00	2	0.4	146	PASS
198	198	100	100	100.0	39510	PASS
199	198	5	9	6.4	2526	PASS
275	198	10	60	24.2	9569	PASS
365	198	1	100	2.5	982	PASS
441	442	0.01	24	15.4	5224	PASS
442	198	50	100	85.9	33923	PASS
443	442	15	24	18.5	6287	PASS