
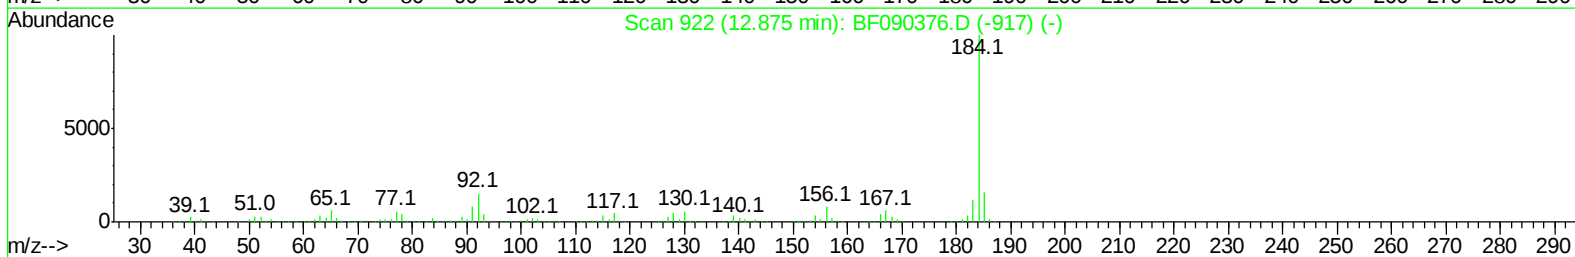
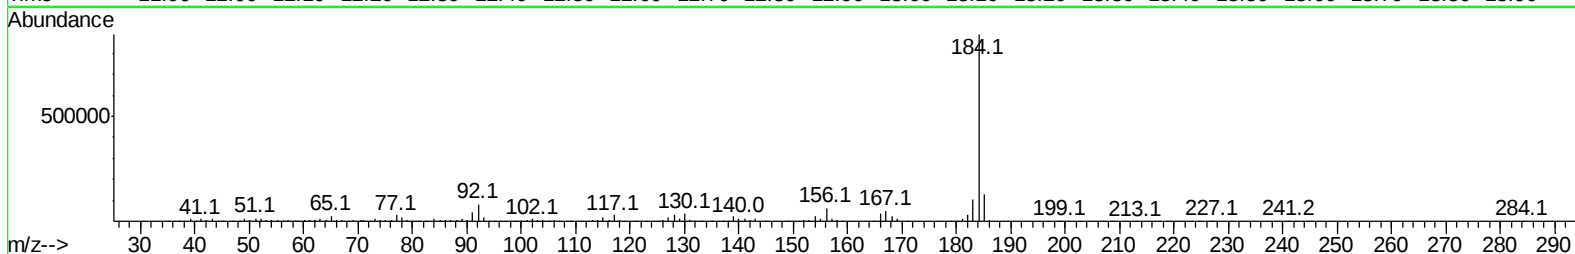


Data Path : Z:\HPCHEM1\BNA F\Data\BF100716\
Data File : BF090437.D
Acq On : 7 Oct 2016 11:16
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 15:06:03 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF100516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 05 14:57:00 2016
Response via : Initial Calibration

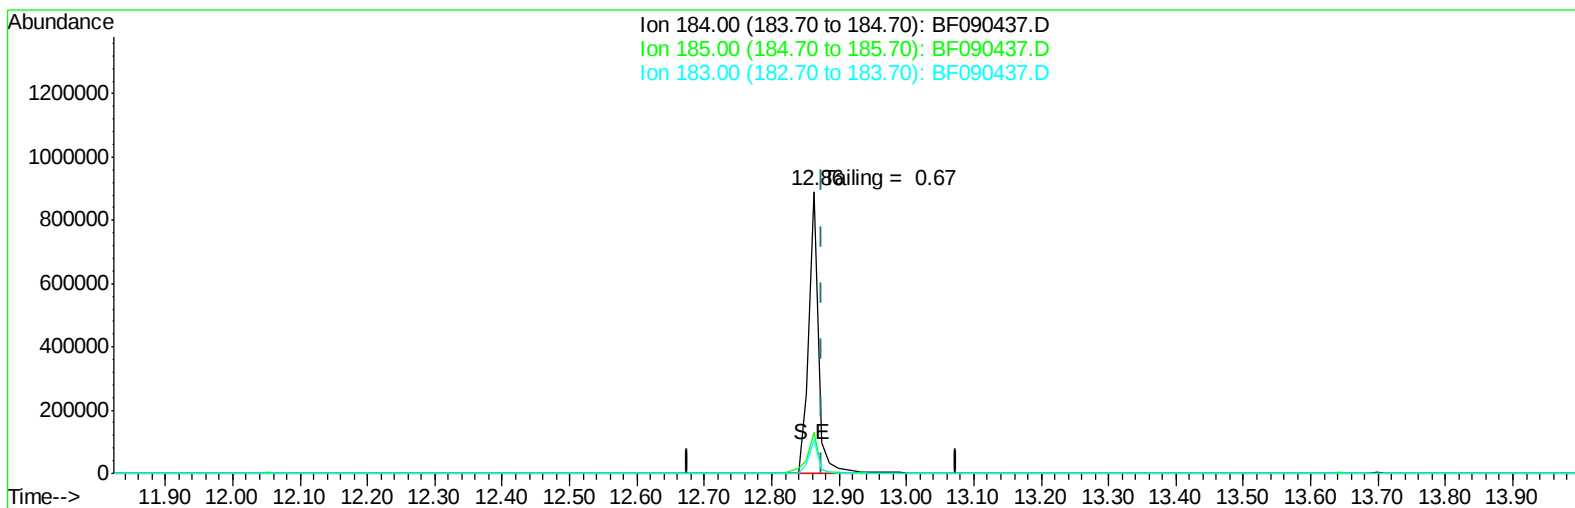

TIC: BF090437.D

(76) Benzidine




12.864min (-0.012) 96513.21ng

response 911026

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.68
183.00	12.00	11.70
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF100716\
Data File : BF090437.D
Acq On : 7 Oct 2016 11:16
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 15:06:03 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF100516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 05 14:57:00 2016
Response via : Initial Calibration

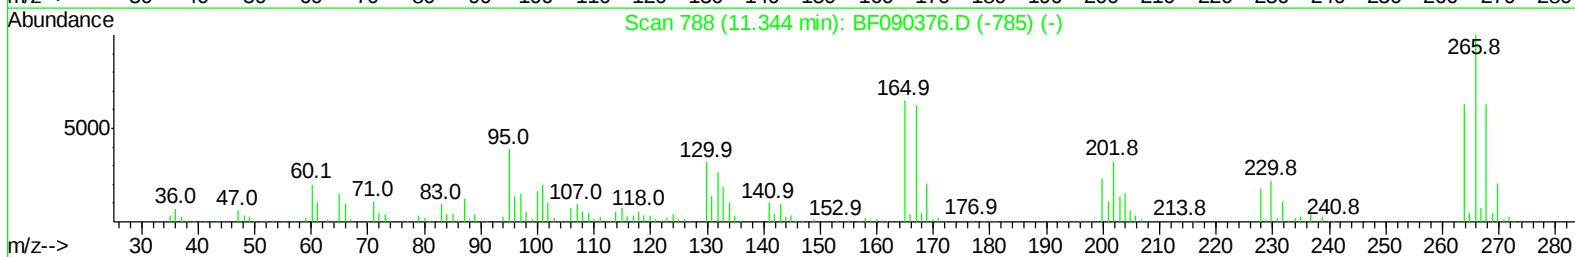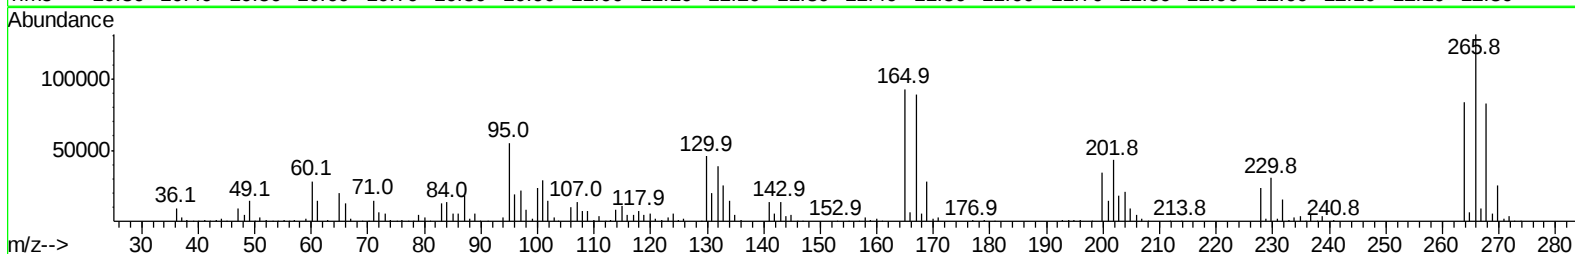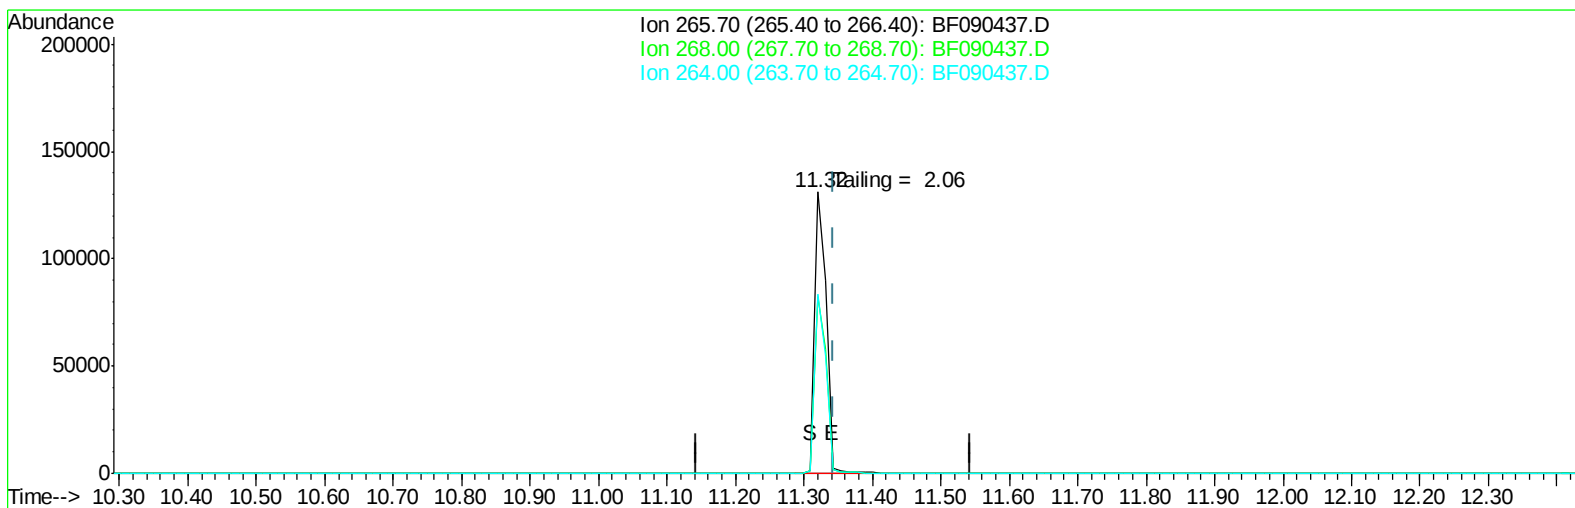

TIC: BF090437.D

(69) Pentachlorophenol (C)

11.321min (-0.023) 0.00ng

response 157462

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	62.91
264.00	64.40	63.78
0.00	0.00	0.00