
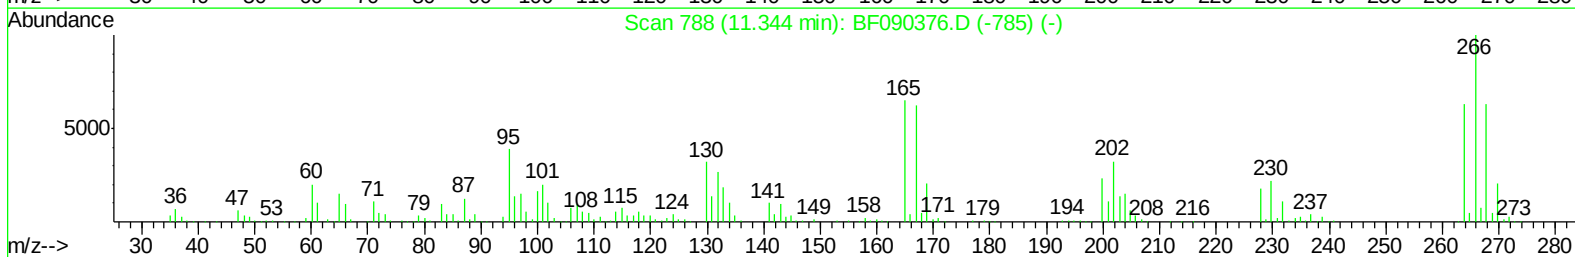
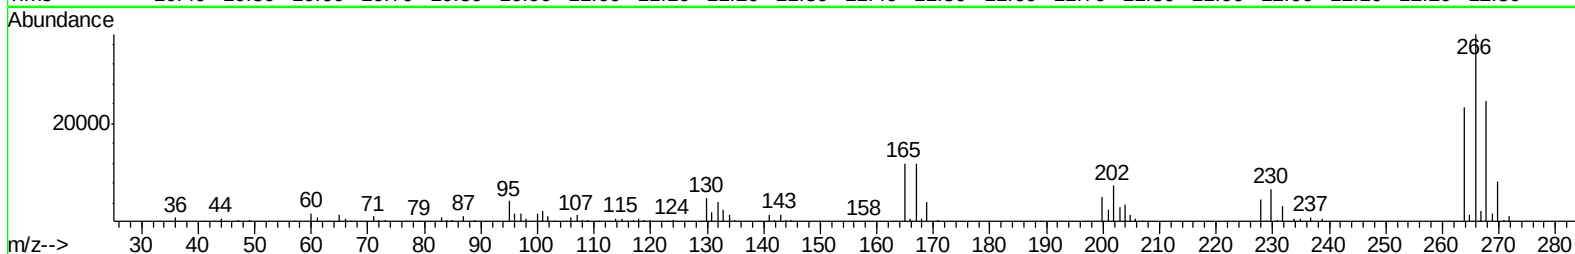


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100716\
Data File : BF090461.D
Acq On : 8 Oct 2016 1:08
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 04:14:00 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF100516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 05 14:57:00 2016
Response via : Initial Calibration

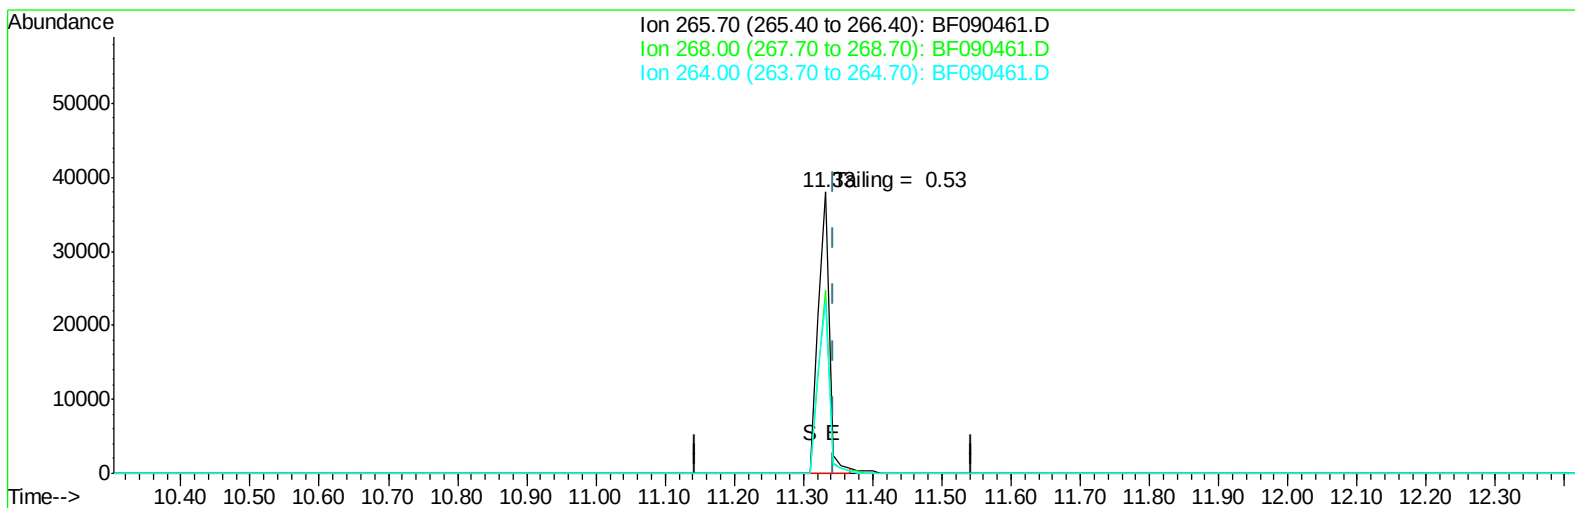

TIC: BF090461.D

(69) Pentachlorophenol (C)




11.332min (-0.012) 0.00ng

response 44070

Ion	Exp%	Act%
265.70	100	100
268.00	63.60	65.03
264.00	64.40	61.05
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100716\
Data File : BF090461.D
Acq On : 8 Oct 2016 1:08
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 04:14:00 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF100516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 05 14:57:00 2016
Response via : Initial Calibration

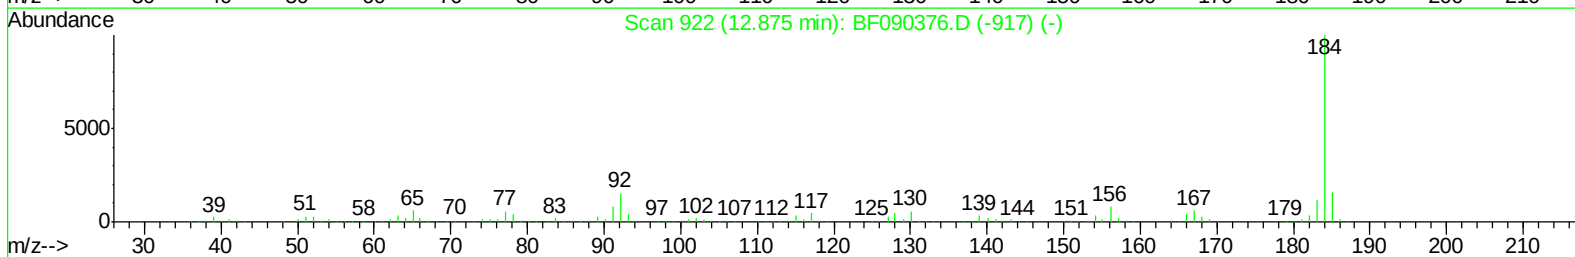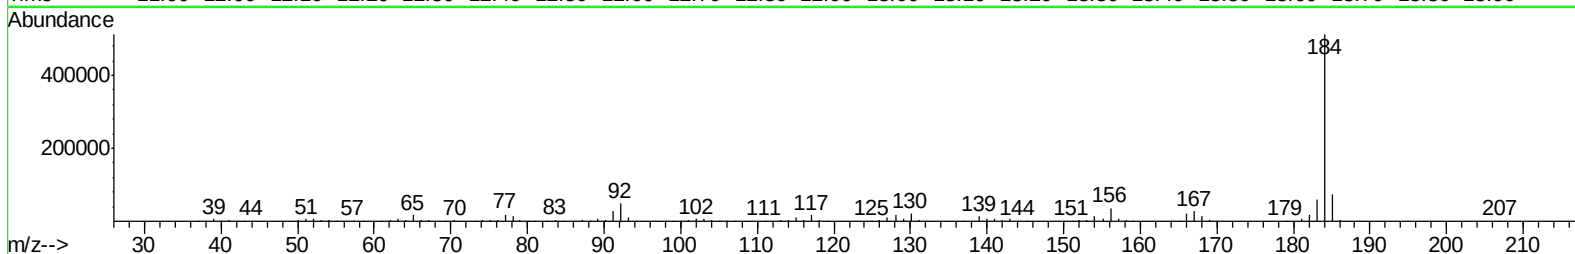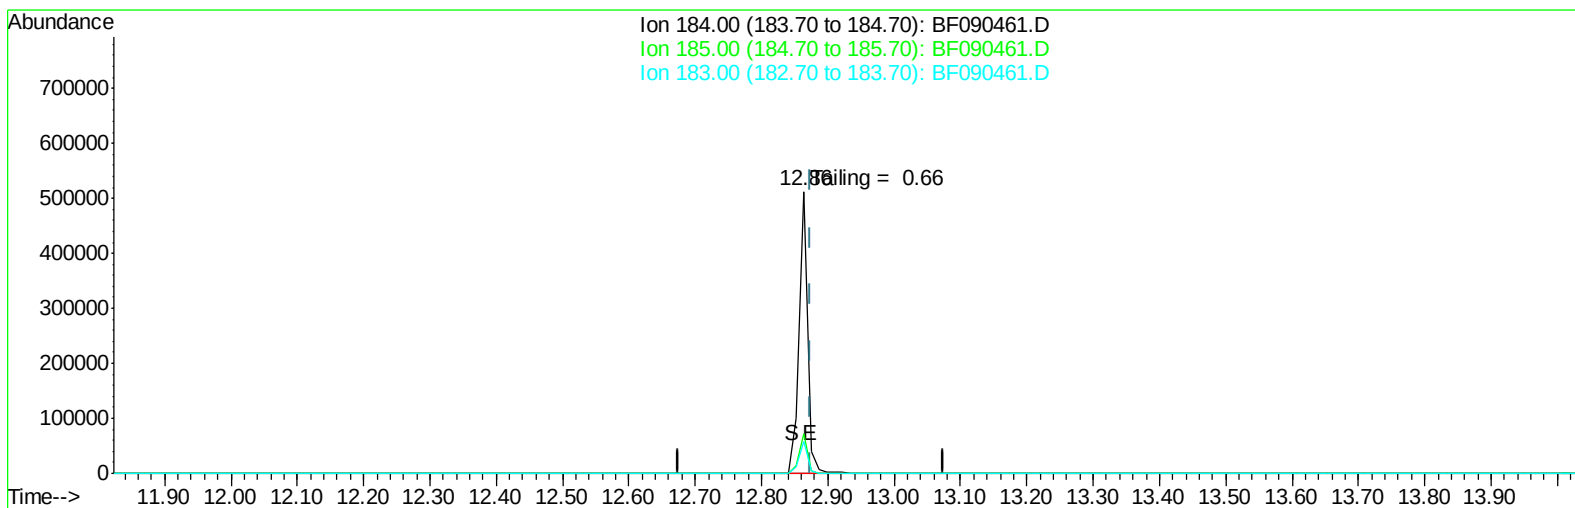

TIC: BF090461.D

(76) Benzidine

12.863min (-0.012) 0.00ng

response 460637

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.27
183.00	12.00	11.40
0.00	0.00	0.00