


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100716\
 Data File : BF090437.D
 Acq On : 7 Oct 2016 11:16
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF100516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 05 14:57:00 2016

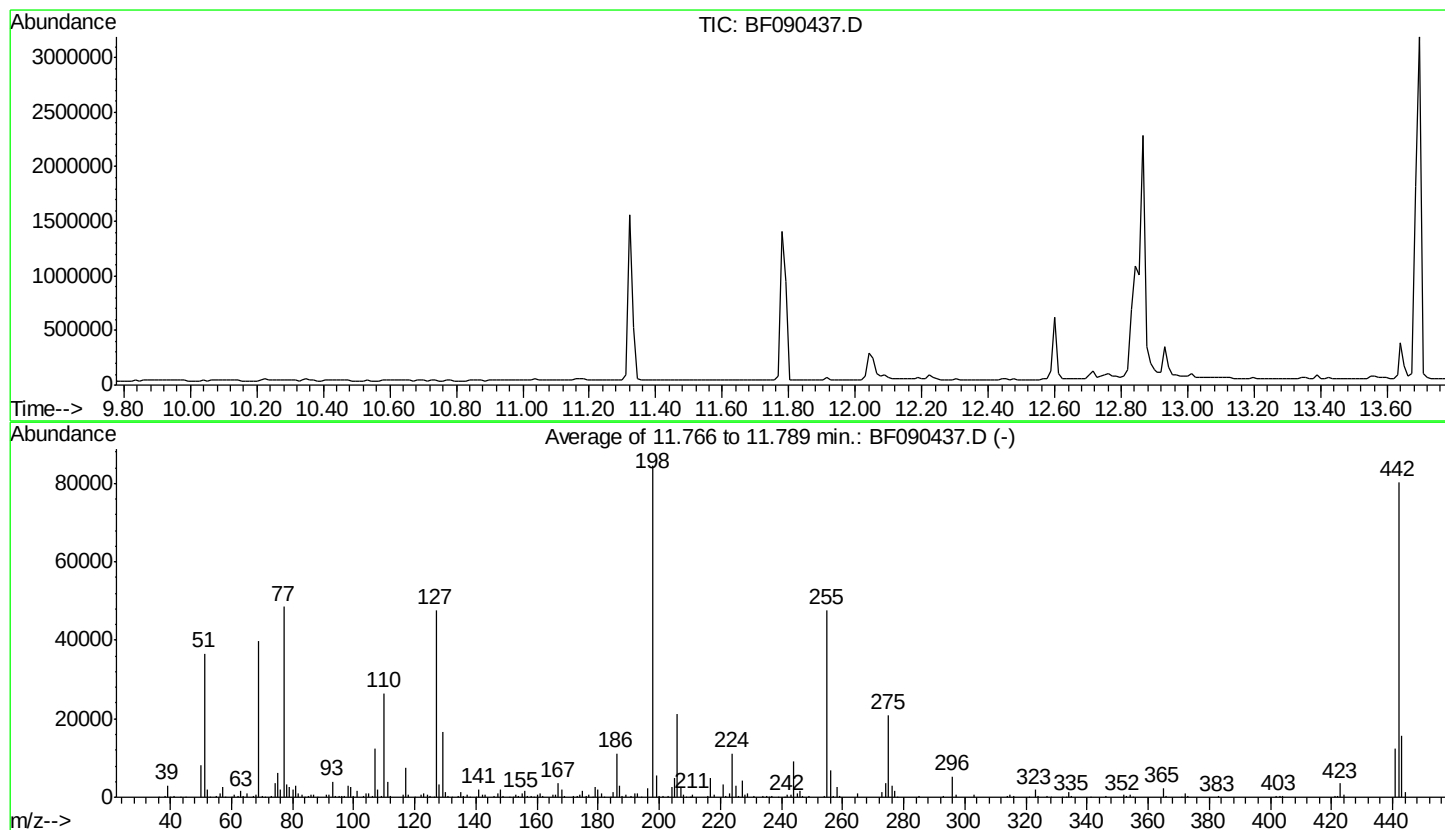

AutoFind: Scans 825, 826, 827; Background Corrected with Scan 822

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.3	36615	PASS
68	69	0.00	2	1.5	613	PASS
69	198	0.00	100	46.9	39658	PASS
70	69	0.00	2	1.0	398	PASS
127	198	10	80	56.5	47714	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	84515	PASS
199	198	5	9	6.7	5639	PASS
275	198	10	60	24.8	20973	PASS
365	198	1	100	2.8	2335	PASS
441	442	0.01	24	15.6	12507	PASS
442	198	50	100	95.0	80264	PASS
443	442	15	24	19.5	15616	PASS