


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100716\
 Data File : BF090461.D
 Acq On : 8 Oct 2016 1:08
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF100516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 05 14:57:00 2016

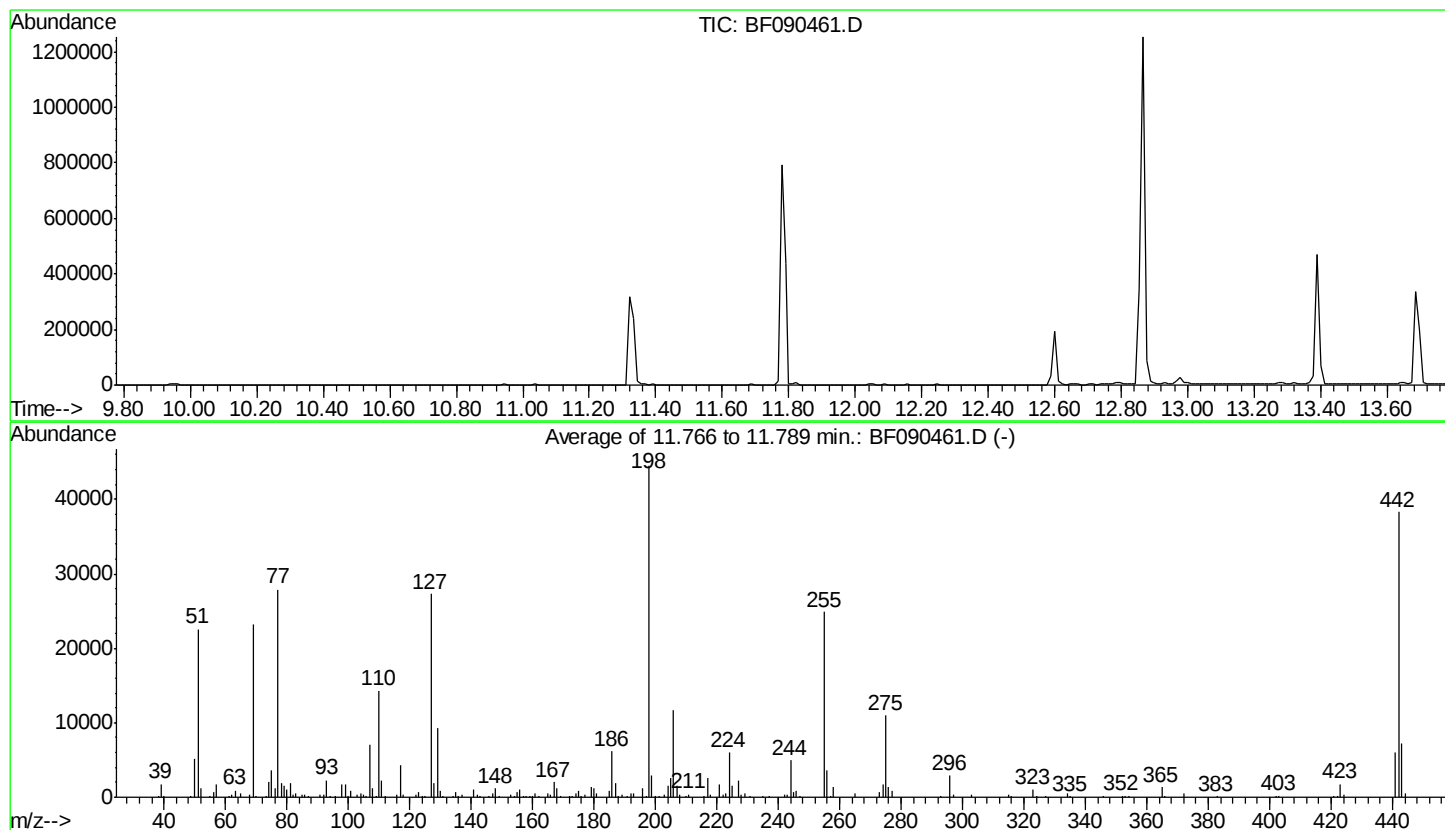

AutoFind: Scans 825, 826, 827; Background Corrected with Scan 822

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.6	22535	PASS
68	69	0.00	2	1.4	321	PASS
69	198	0.00	100	52.0	23150	PASS
70	69	0.00	2	0.6	135	PASS
127	198	10	80	61.3	27298	PASS
197	198	0.00	2	0.2	110	PASS
198	198	100	100	100.0	44533	PASS
199	198	5	9	6.6	2941	PASS
275	198	10	60	24.6	10944	PASS
365	198	1	100	2.9	1306	PASS
441	442	0.01	24	15.7	6006	PASS
442	198	50	100	86.1	38337	PASS
443	442	15	24	18.9	7243	PASS