

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100717\
 Data File : BF099197.D
 Acq On : 7 Oct 2017 16:35
 Operator : SJ/JU
 Sample : I5586-13 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G54B-0-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.075	505	508	516	rBV	53505	52663	5.91%	0.685%
2	5.475	573	576	587	rBV	333505	315307	35.39%	4.104%
3	6.492	745	749	760	rBV	323350	325888	36.58%	4.241%
4	6.634	769	773	776	rBV	417495	344347	38.65%	4.482%
5	6.863	808	812	816	rBV	910297	716080	80.37%	9.320%
6	7.016	835	838	842	rBV	318729	269971	30.30%	3.514%
7	7.422	904	907	911	rBV	235685	179711	20.17%	2.339%
8	8.145	1026	1030	1033	rBV	1166205	890942	100.00%	11.595%
9	8.728	1123	1129	1133	rVB3	11456	11222	1.26%	0.146%
10	9.216	1209	1212	1219	rBV	470185	356256	39.99%	4.637%
11	9.292	1221	1225	1228	rBV	17461	14273	1.60%	0.186%
12	9.610	1276	1279	1282	rBV	51062	40388	4.53%	0.526%
13	9.822	1311	1315	1318	rBV	17764	15814	1.77%	0.206%
14	9.898	1325	1328	1332	rBV	893324	833287	93.53%	10.845%
15	9.933	1332	1334	1338	rVB	12120	11659	1.31%	0.152%
16	10.322	1397	1400	1403	rVB	23078	18643	2.09%	0.243%
17	10.539	1434	1437	1444	rVB3	10283	11599	1.30%	0.151%
18	10.686	1459	1462	1469	rVB	129200	109114	12.25%	1.420%
19	10.792	1477	1480	1489	rVB3	24864	41391	4.65%	0.539%
20	11.239	1551	1556	1558	rBV	25794	20953	2.35%	0.273%
21	11.269	1558	1561	1568	rVB6	13809	21044	2.36%	0.274%
22	11.386	1577	1581	1584	rBV	842906	707467	79.41%	9.207%
23	11.410	1584	1585	1588	rVV	95937	57461	6.45%	0.748%
24	11.463	1591	1594	1596	rVB	26661	19927	2.24%	0.259%
25	11.669	1626	1629	1632	rBV	17169	14928	1.68%	0.194%
26	11.886	1662	1666	1669	rBV	14588	21265	2.39%	0.277%
27	11.916	1669	1671	1674	rVB	20907	18288	2.05%	0.238%
28	11.998	1682	1685	1687	rBV2	17626	14251	1.60%	0.185%
29	12.021	1687	1689	1692	rVB	15008	12559	1.41%	0.163%
30	12.074	1695	1698	1702	rBV2	23075	23200	2.60%	0.302%
31	12.180	1712	1716	1719	rBV4	18350	21782	2.44%	0.283%
32	12.216	1719	1722	1726	rVV5	11192	16752	1.88%	0.218%
33	12.310	1736	1738	1743	rBV5	11871	19608	2.20%	0.255%
34	12.363	1743	1747	1749	rVV3	10961	13698	1.54%	0.178%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100717\
Data File : BF099197.D
Acq On : 7 Oct 2017 16:35
Operator : SJ/JU
Sample : I5586-13 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G54B-0-3

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.433	1757	1759	1761	rBV	15687	12566	1.41%	0.164%
36	12.463	1761	1764	1768	rVB3	25653	23903	2.68%	0.311%
37	12.521	1772	1774	1777	rBV3	12966	15885	1.78%	0.207%
38	12.598	1784	1787	1792	rBV	134923	116940	13.13%	1.522%
39	12.645	1792	1795	1797	rVV3	10905	11513	1.29%	0.150%
40	12.692	1801	1803	1806	rBV2	12307	16180	1.82%	0.211%
41	12.751	1811	1813	1815	rBV3	14236	13322	1.50%	0.173%
42	12.833	1821	1827	1828	rBV2	186191	228327	25.63%	2.972%
43	12.845	1828	1829	1834	rVB	244308	225183	25.27%	2.931%
44	12.963	1846	1849	1852	rVB	277175	236284	26.52%	3.075%
45	13.186	1885	1887	1890	rBV3	20945	25909	2.91%	0.337%
46	14.027	2026	2030	2033	rBV	717168	664910	74.63%	8.654%
47	15.504	2277	2281	2286	rVB	421854	531010	59.60%	6.911%


Sum of corrected areas: 7683670

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100717\
Data File : BF099197.D
Acq On : 7 Oct 2017 16:35
Operator : SJ/JU
Sample : I5586-13 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G54B-0-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

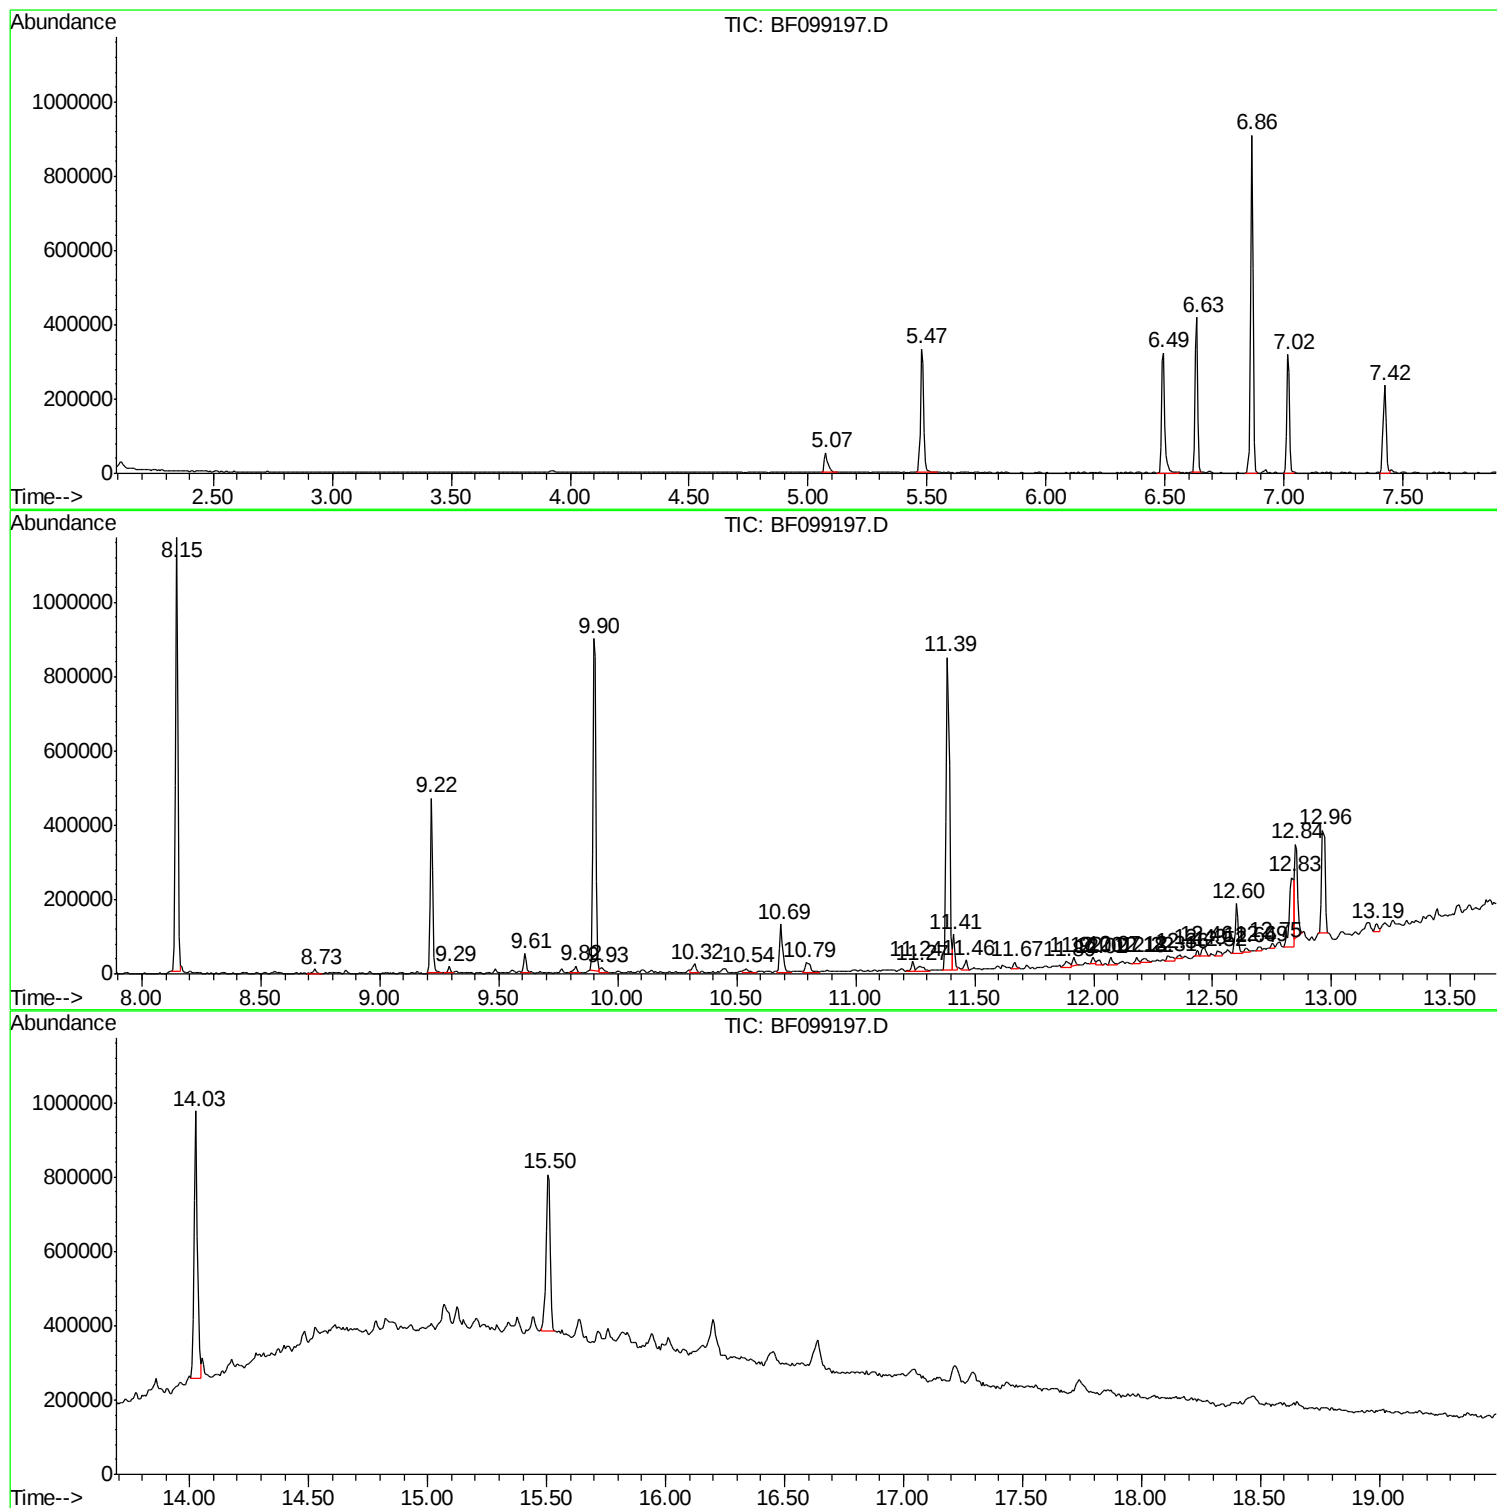

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100717\
Data File : BF099197.D
Acq On : 7 Oct 2017 16:35
Operator : SJ/JU
Sample : I5586-13 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G54B-0-3










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.63 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.63	9.62 ng	344347	1,4-Dichlorobenzene-d4	6.86

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Xenon	132	Xe	007440-63-3	9
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

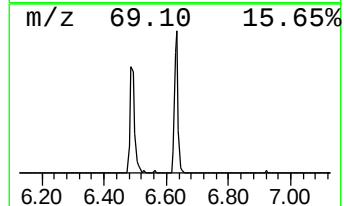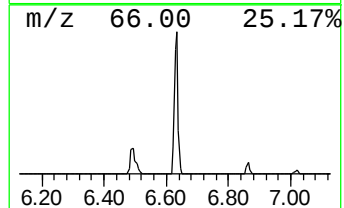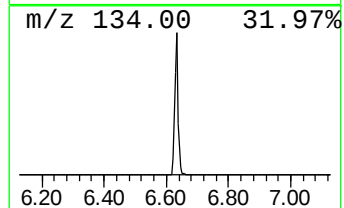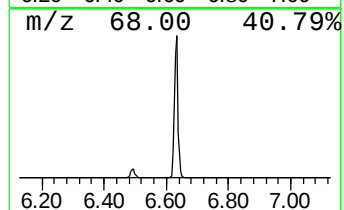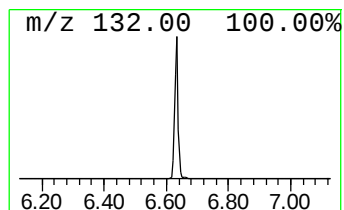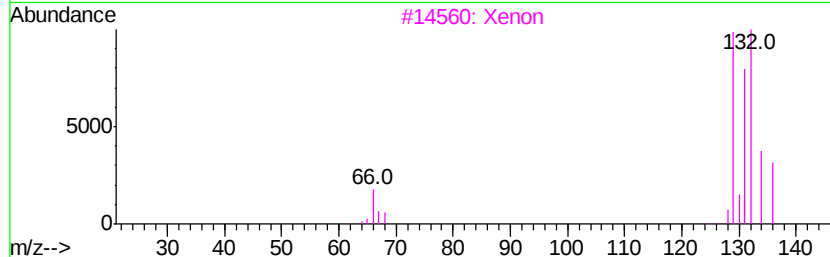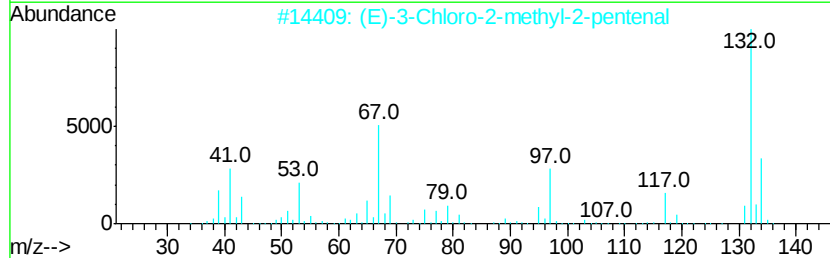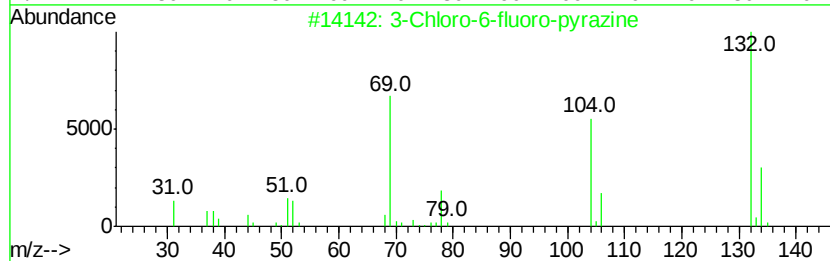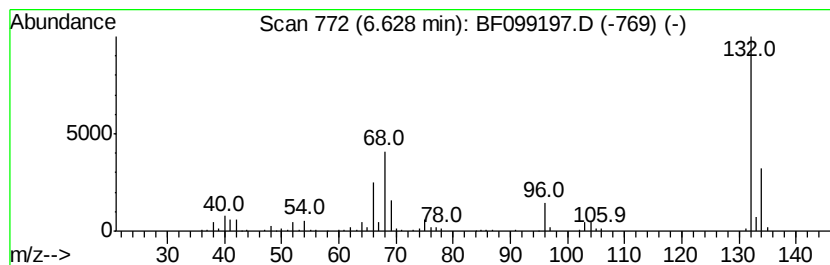

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100717\
Data File : BF099197.D
Acq On : 7 Oct 2017 16:35
Operator : SJ/JU
Sample : I5586-13 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G54B-0-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.63	6.63	9.6	ng	344347	1	6.86	716080	20.0