


Data Path : Z:\HPCHEM1\BNA F\Data\BF100717\
 Data File : BF099184.D
 Acq On : 7 Oct 2017 10:25
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 05 17:20:48 2017

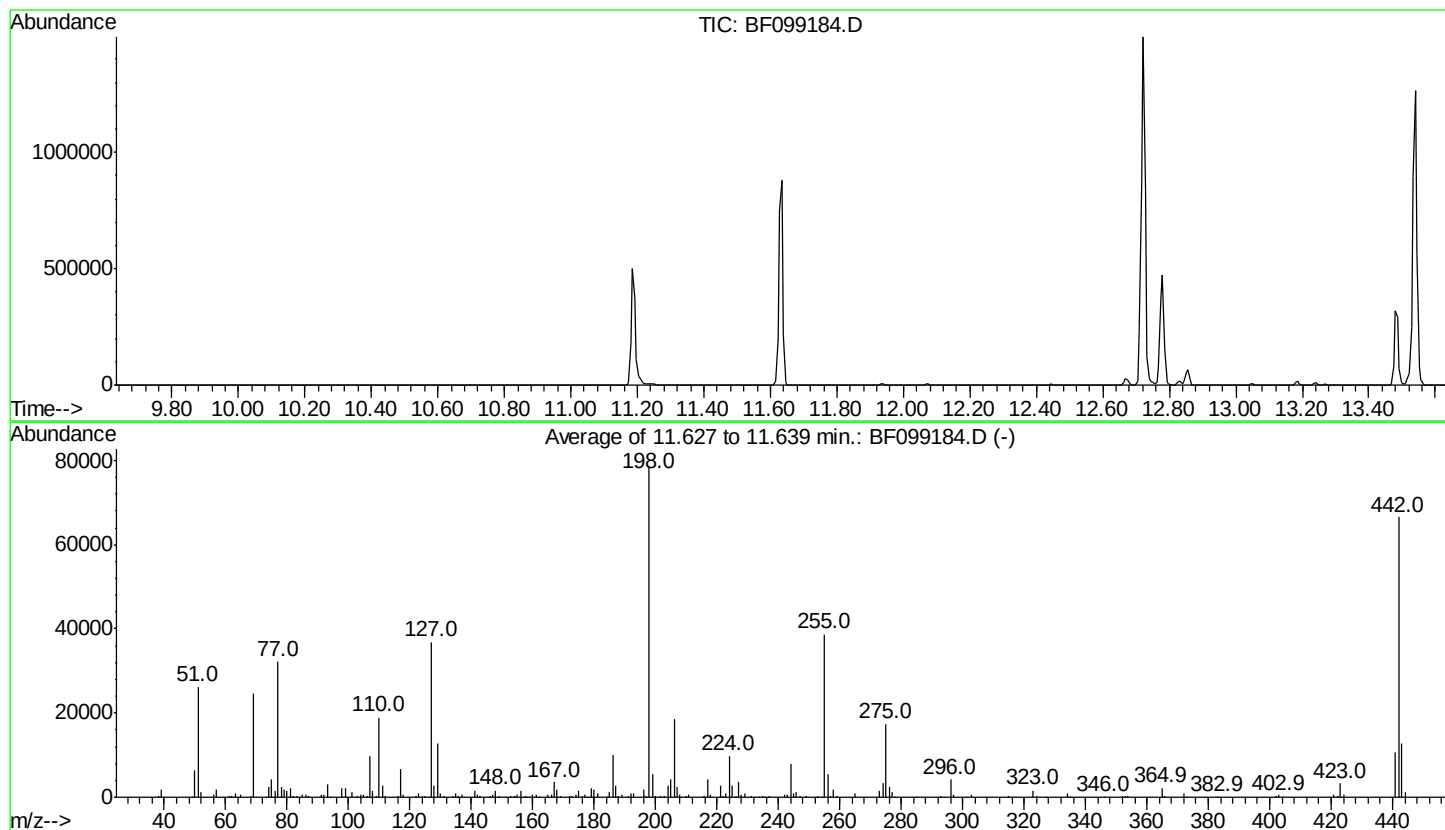

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	26222	PASS
68	69	0.00	2	1.8	447	PASS
69	198	0.00	100	31.4	24738	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.9	36914	PASS
197	198	0.00	2	0.5	385	PASS
198	198	100	100	100.0	78778	PASS
199	198	5	9	6.8	5333	PASS
275	198	10	60	22.2	17489	PASS
365	198	1	100	2.8	2173	PASS
441	442	0.01	24	15.8	10522	PASS
442	198	50	100	84.5	66549	PASS
443	442	15	24	19.1	12725	PASS