


Data Path : Z:\HPCHEM1\BNA F\Data\BF100717\
 Data File : BF099210.D
 Acq On : 7 Oct 2017 23:38
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 05 17:20:48 2017

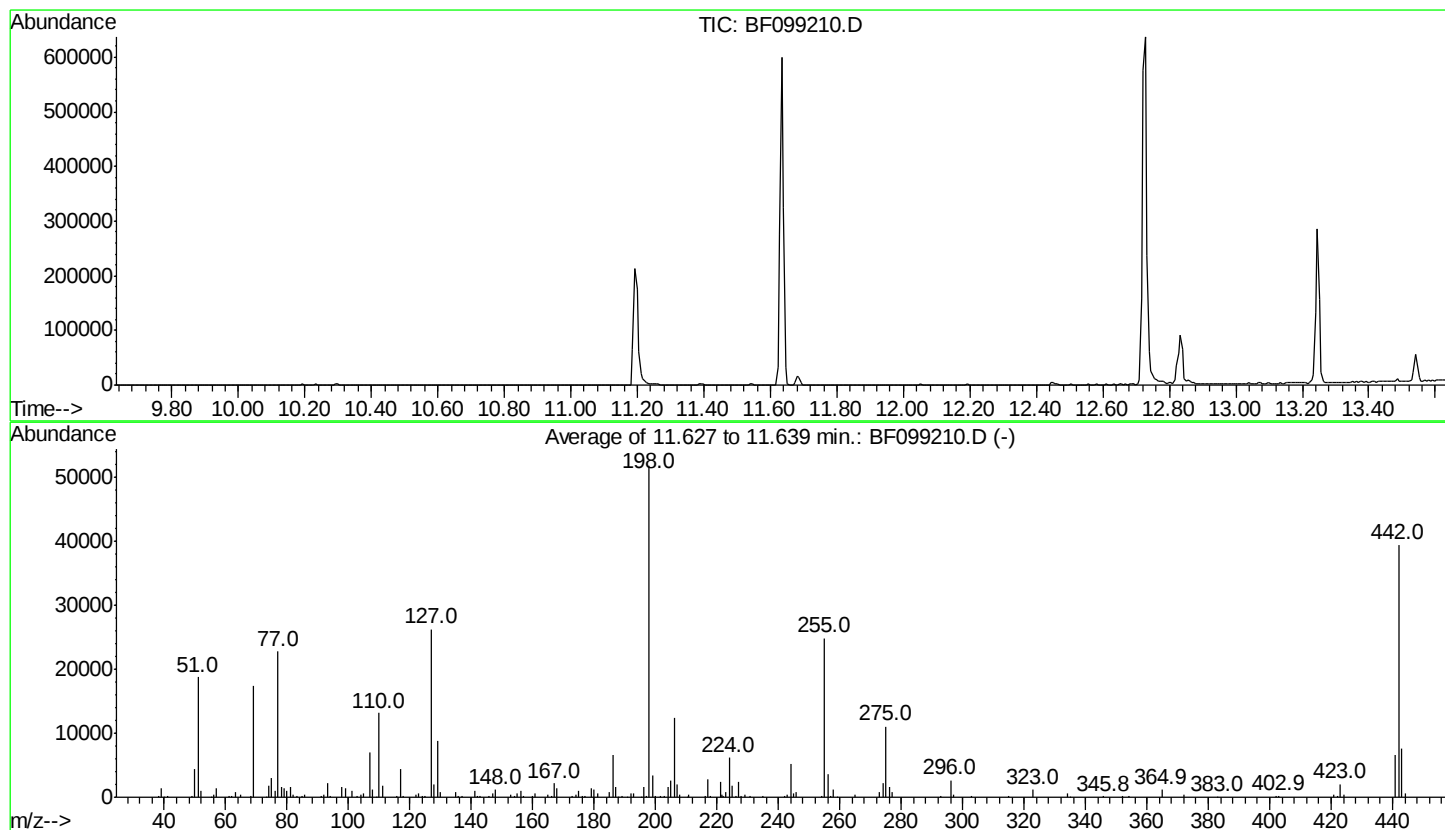

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	18742	PASS
68	69	0.00	2	0.8	143	PASS
69	198	0.00	100	33.5	17300	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.8	26258	PASS
197	198	0.00	2	0.5	255	PASS
198	198	100	100	100.0	51717	PASS
199	198	5	9	6.7	3485	PASS
275	198	10	60	21.3	11023	PASS
365	198	1	100	2.2	1137	PASS
441	442	0.01	24	16.5	6518	PASS
442	198	50	100	76.2	39412	PASS
443	442	15	24	19.4	7660	PASS