


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF100720\
 Data File : BF121863.D
 Acq On : 7 Oct 2020 8:47
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 01 14:29:14 2020

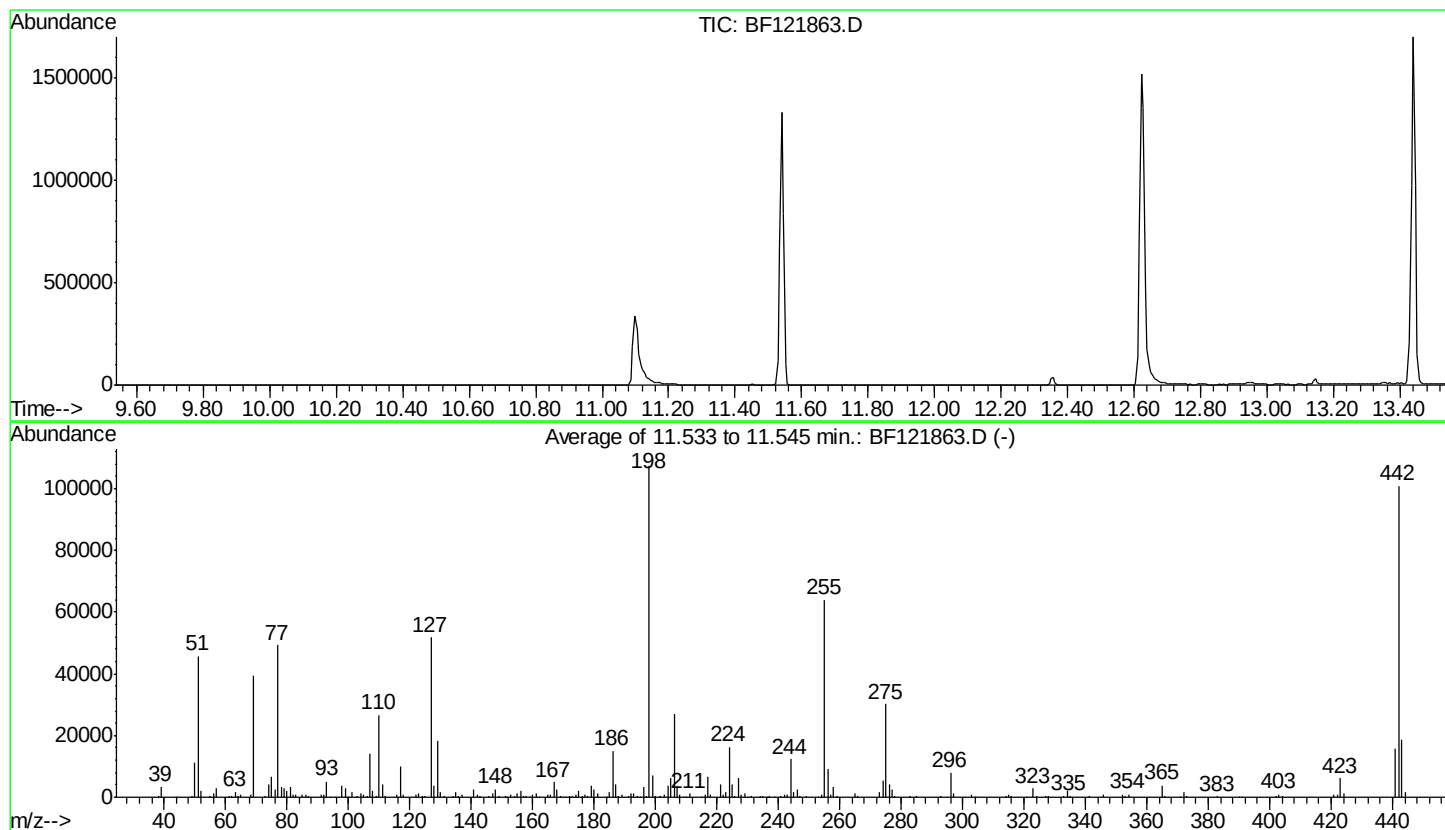

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	45685	PASS
68	69	0.00	2	1.6	647	PASS
69	198	0.00	100	36.7	39496	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.1	51709	PASS
197	198	0.00	2	0.5	572	PASS
198	198	100	100	100.0	107488	PASS
199	198	5	9	6.7	7185	PASS
275	198	10	60	28.2	30266	PASS
365	198	1	100	3.6	3841	PASS
441	198	0.01	100	14.5	15603	PASS
442	198	50	100	93.9	100909	PASS
443	442	15	24	18.4	18526	PASS