
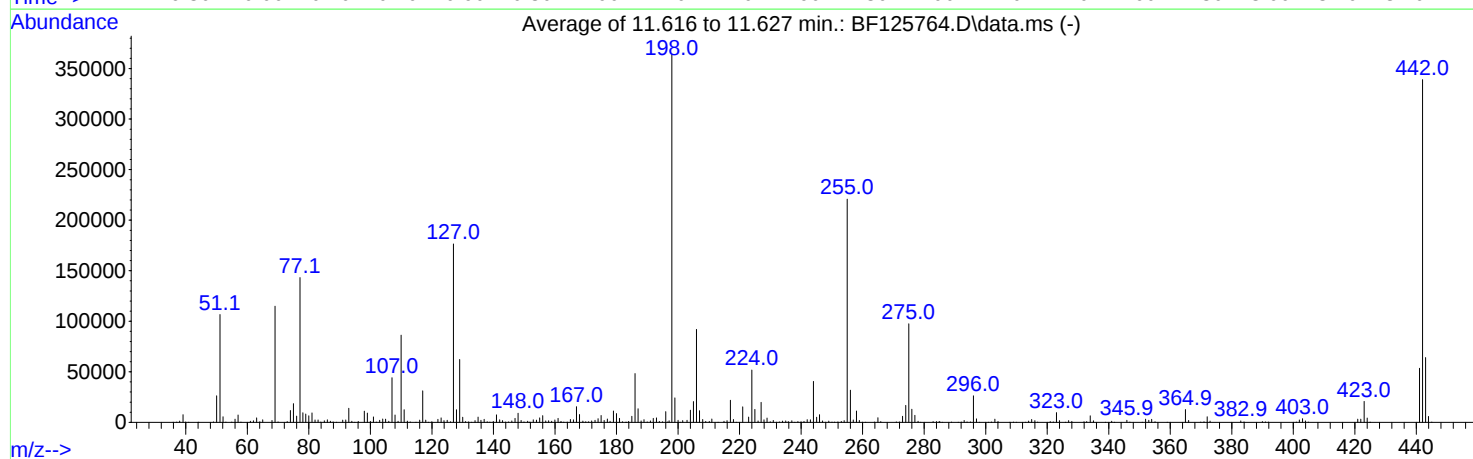


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100721\
 Data File : BF125764.D
 Acq On : 7 Oct 2021 11:57
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 07 17:16:23 2021

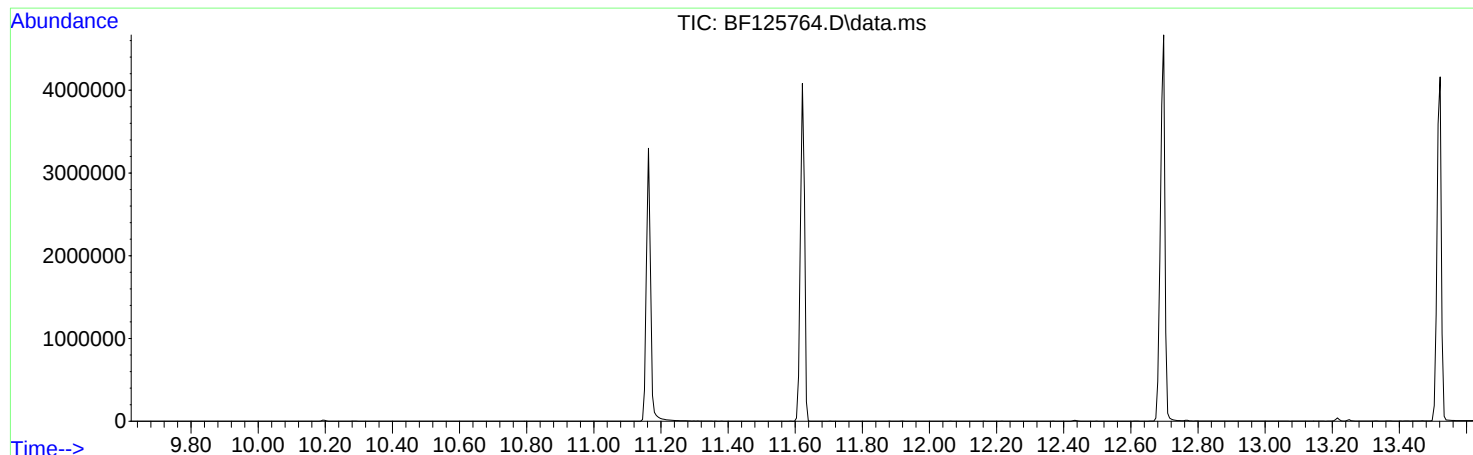




AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.3	106763	PASS
68	69	0.00	2	1.7	1903	PASS
69	198	0.00	100	31.6	114952	PASS
70	69	0.00	2	0.4	482	PASS
127	198	10	80	48.5	176429	PASS
197	198	0.00	2	0.4	1545	PASS
198	198	100	100	100.0	363861	PASS
199	198	5	9	6.7	24296	PASS
275	198	10	60	26.8	97448	PASS
365	198	1	100	3.5	12676	PASS
441	198	0.01	100	14.7	53424	PASS
442	442	50	100	100.0	339051	PASS
443	442	15	24	18.9	64064	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100721\
 Data File : BF125764.D
 Acq On : 7 Oct 2021 11:57
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 07 18:42:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 07 17:16:23 2021
 Response via : Initial Calibration

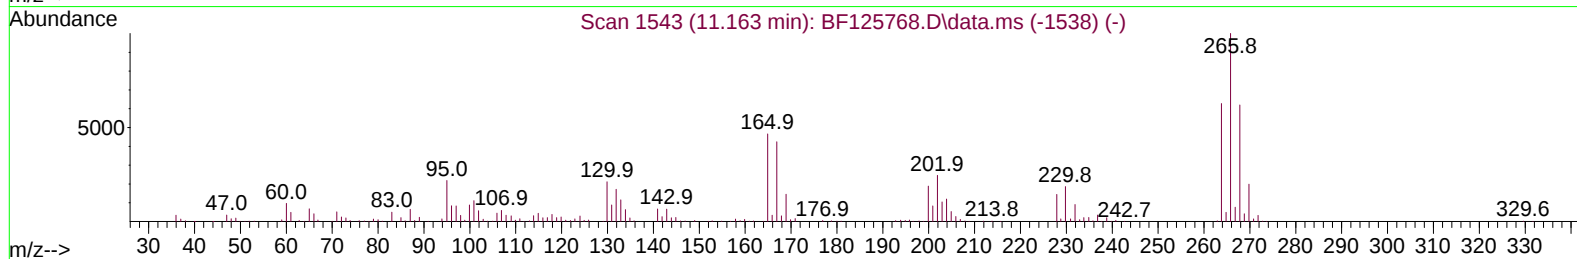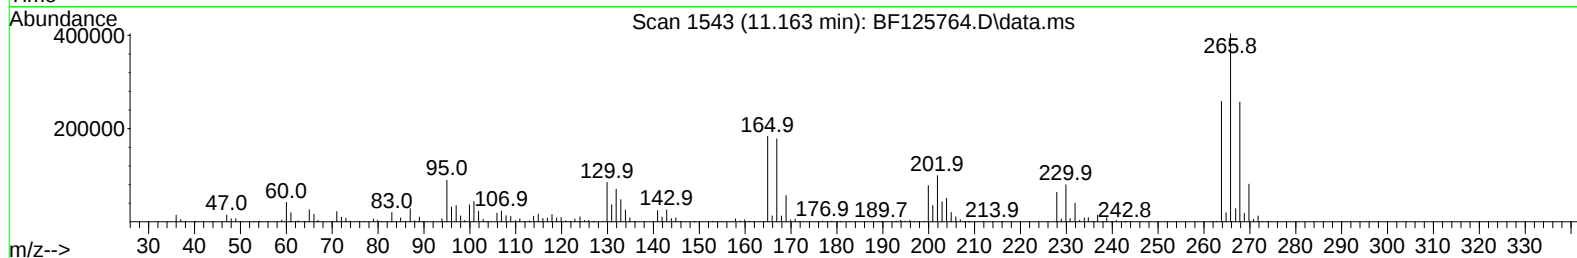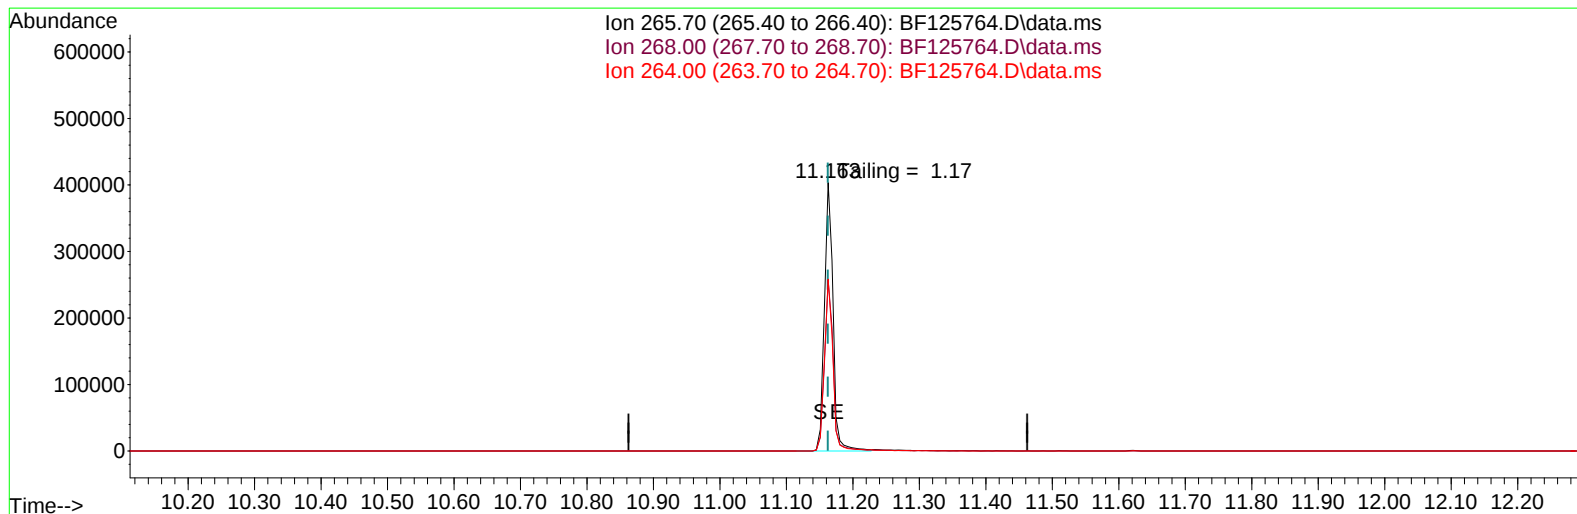

TIC: BF125764.D\data.ms

(70) Pentachlorophenol (C)

11.163min (+ 0.000) 33992.74 ng




response 368315

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	63.66
264.00	69.90	64.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100721\
 Data File : BF125764.D
 Acq On : 7 Oct 2021 11:57
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 07 18:42:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 07 17:16:23 2021
 Response via : Initial Calibration

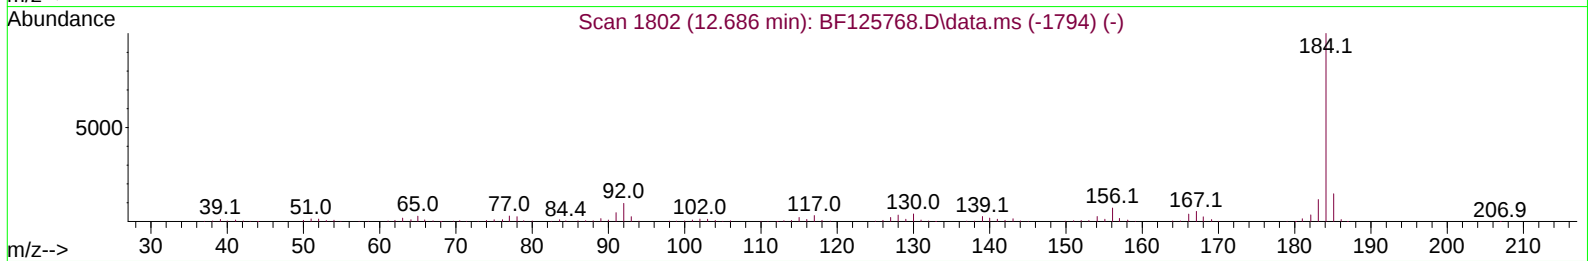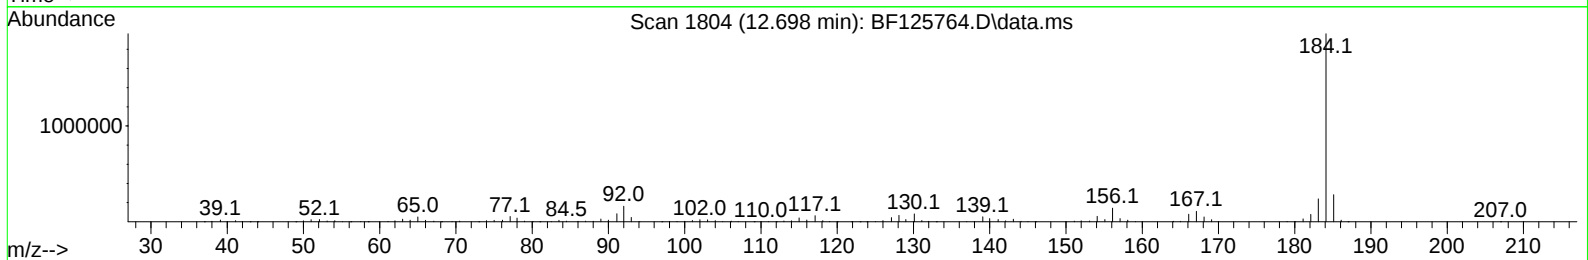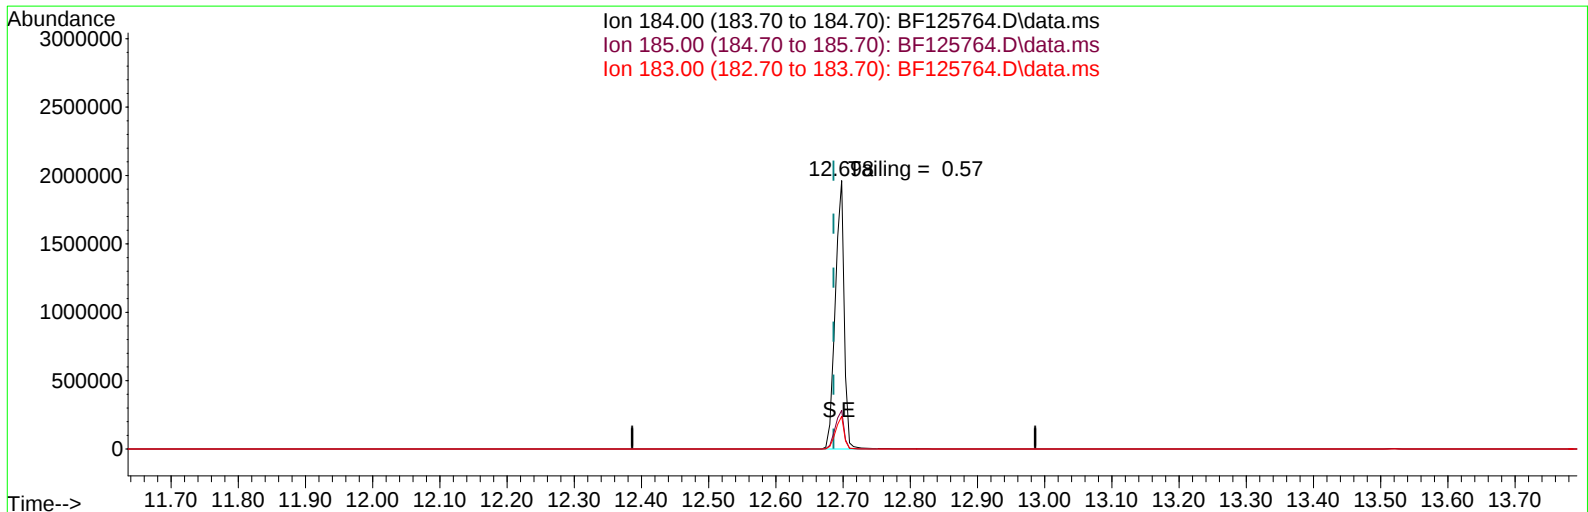

TIC: BF125764.D\data.ms

(77) Benzidine

12.698min (+ 0.012) 0.00 ng

response 1811000

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.39
183.00	10.10	12.20#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/7/2021	BNA_F	<u>BF125764.D</u>
Compound Name	Response	Retention Time
DDT	700994	13.52
DDD	6707	13.21
DDE	148	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6855	707849	0.97