
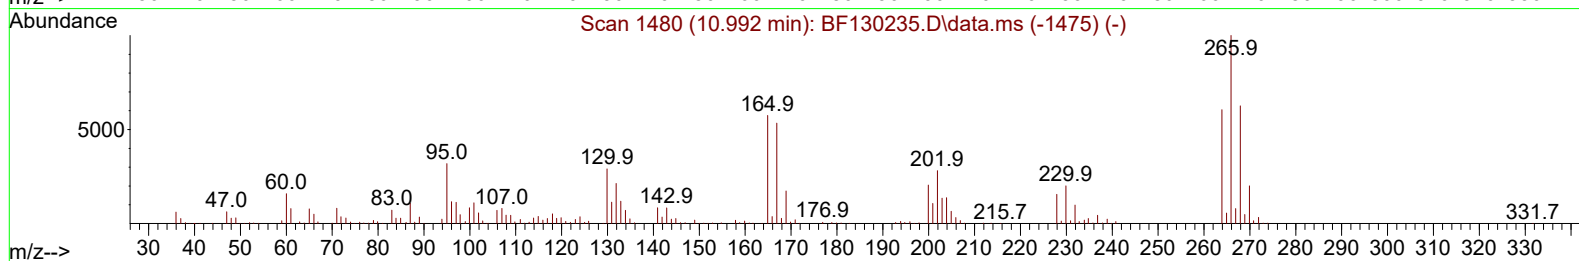
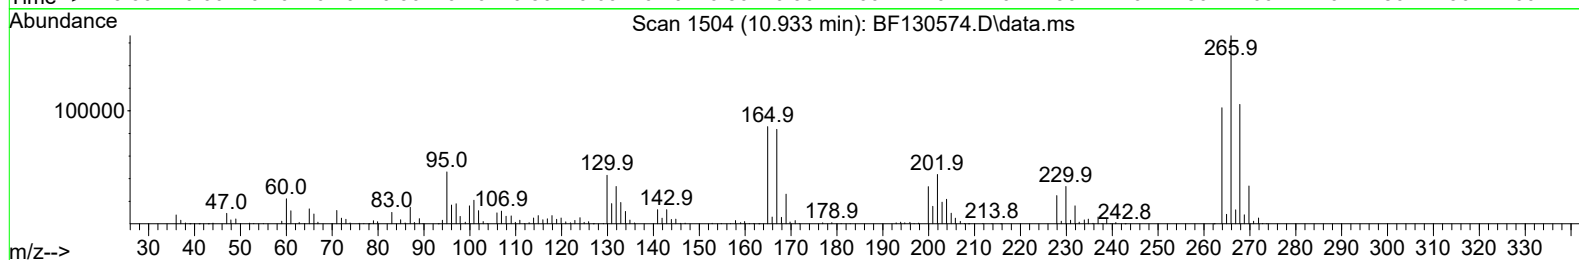


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100722\
 Data File : BF130574.D
 Acq On : 07 Oct 2022 14:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 10 04:11:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 07 02:06:46 2022
 Response via : Initial Calibration

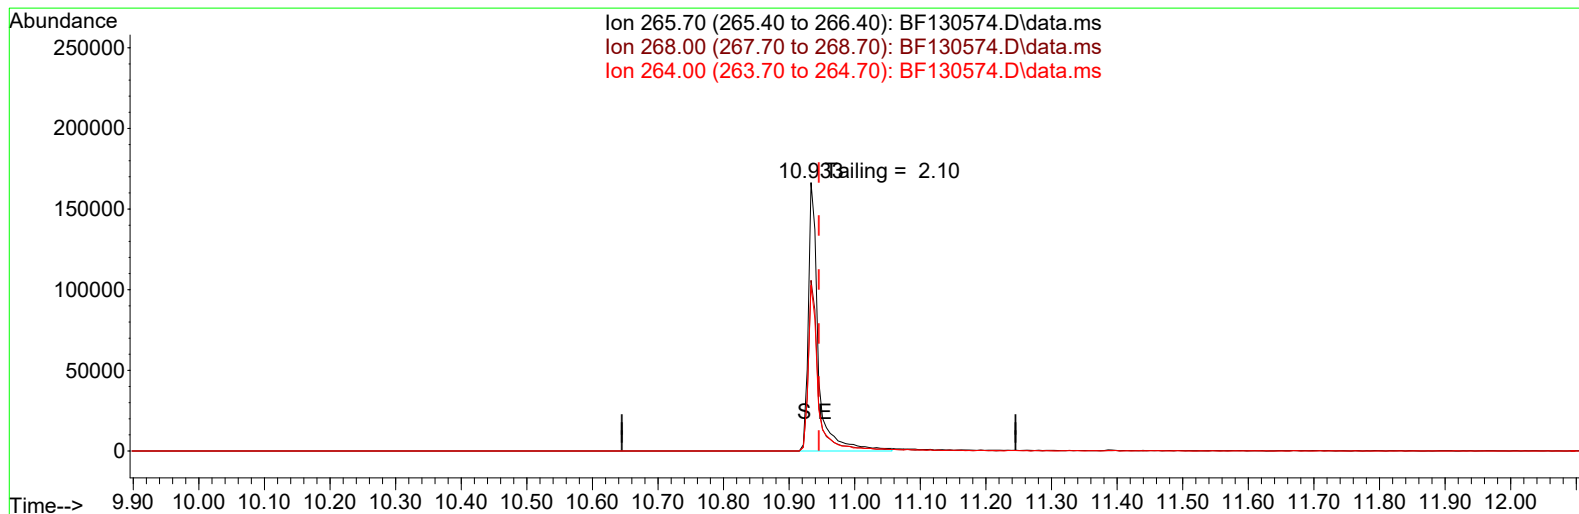

TIC: BF130574.D\data.ms

(70) Pentachlorophenol (C)




10.933min (-0.012) 456180.00 ng

response 180633

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.54
264.00	63.10	61.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100722\
Data File : BF130574.D
Acq On : 07 Oct 2022 14:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 10 04:11:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 07 02:06:46 2022
Response via : Initial Calibration

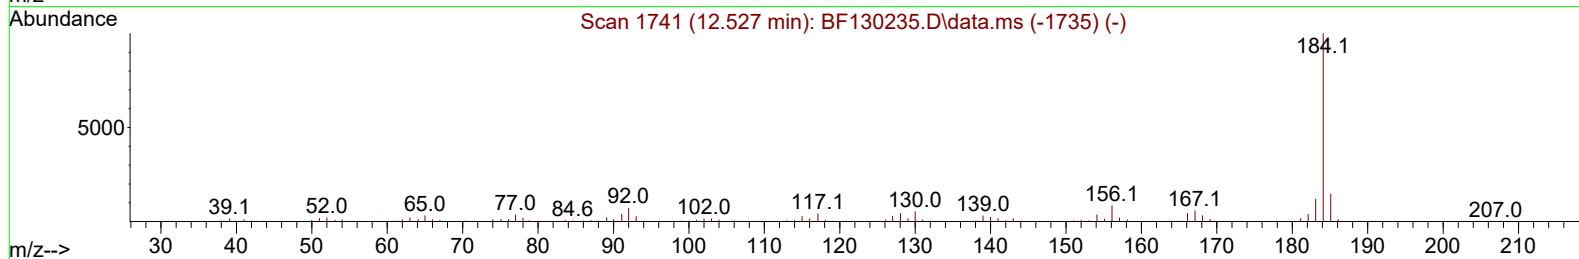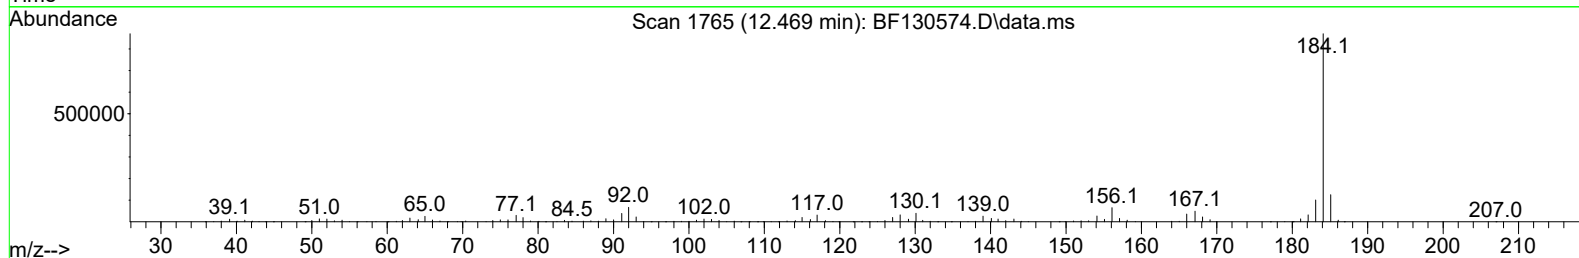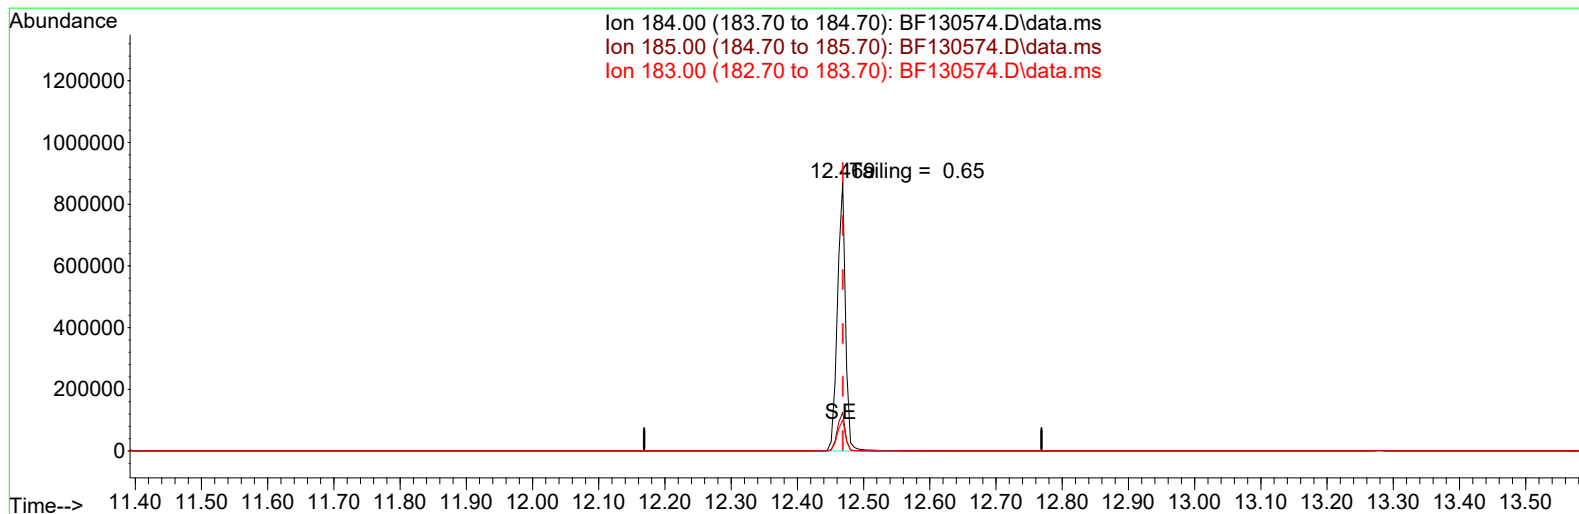

TIC: BF130574.D\data.ms

(77) Benzidine

12.469min (-0.000) 113184.94 ng

response 739273

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.40
183.00	11.40	11.61
0.00	0.00	0.00