

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100722\
 Data File : BF130579.D
 Acq On : 07 Oct 2022 17:23
 Operator : CG\JU
 Sample : N5046-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 R-5

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130579.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.787	455	459	476	rBV	430974	595651	21.98%	3.790%
2	5.222	529	533	552	rBV	1945253	2019599	74.53%	12.852%
3	5.622	597	601	610	rBV	47186	41807	1.54%	0.266%
4	6.257	705	709	712	rBV	2331192	2320469	85.64%	14.766%
5	6.610	766	769	773	rBV	615952	508054	18.75%	3.233%
6	7.181	861	866	869	rBV	1663900	1437768	53.06%	9.149%
7	7.839	971	978	984	rBV6	19554	65396	2.41%	0.416%
8	7.892	984	987	991	rVB	1017322	829158	30.60%	5.276%
9	8.969	1166	1170	1174	rBV	2935601	2709646	100.00%	17.243%
10	9.639	1281	1284	1288	rBV	810639	683803	25.24%	4.351%
11	10.427	1415	1418	1437	rVB	1287056	1178547	43.49%	7.500%
12	11.121	1532	1536	1539	rBV	811908	621360	22.93%	3.954%
13	12.710	1801	1806	1809	rBV	1879601	1706261	62.97%	10.858%
14	13.751	1971	1983	1987	rBV	515397	480446	17.73%	3.057%
15	14.527	2109	2115	2119	rBV2	25332	29711	1.10%	0.189%
16	15.133	2213	2218	2222	rBV	445713	487001	17.97%	3.099%




Sum of corrected areas: 15714677

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100722\
Data File : BF130579.D
Acq On : 07 Oct 2022 17:23
Operator : CG\JU
Sample : N5046-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
R-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

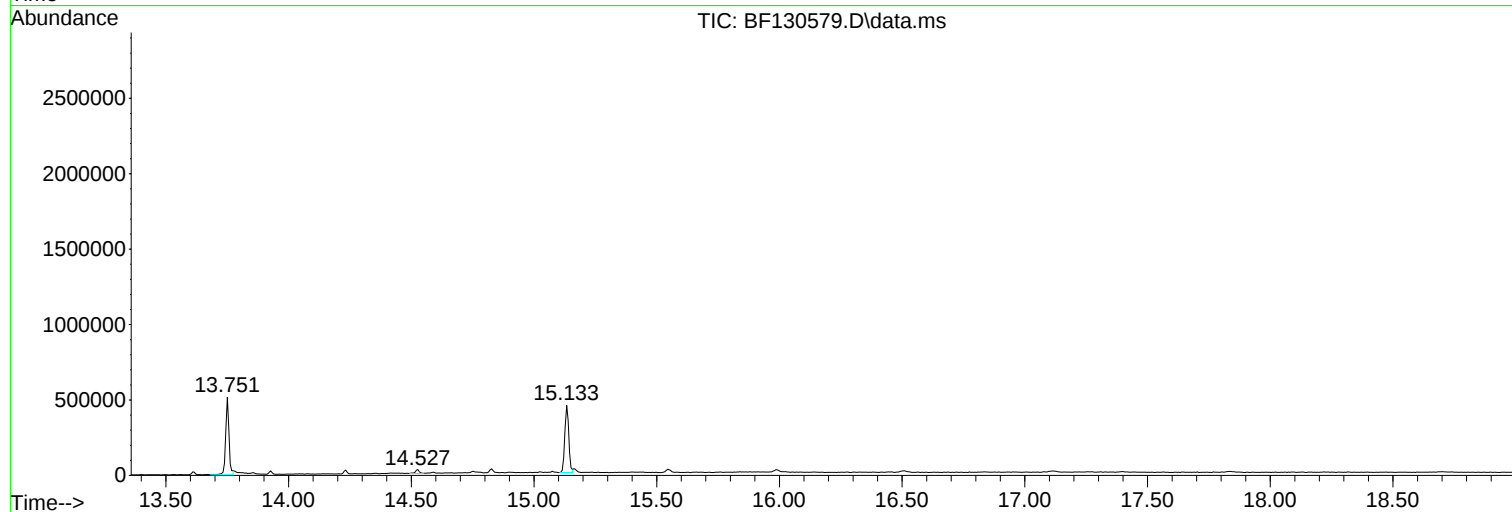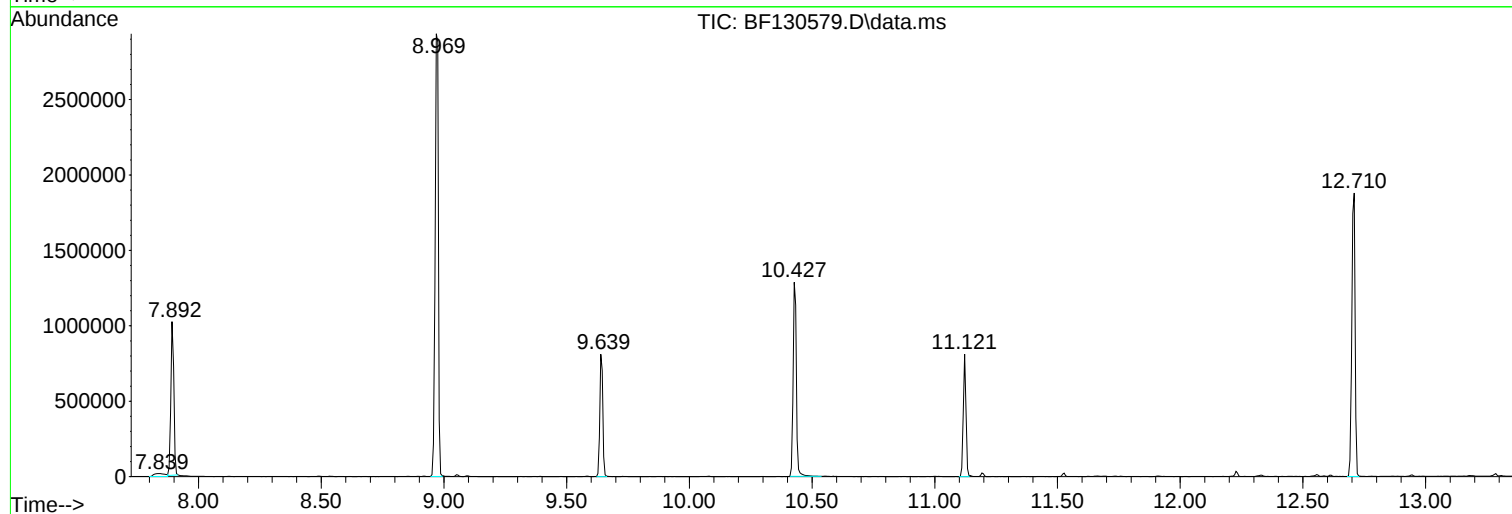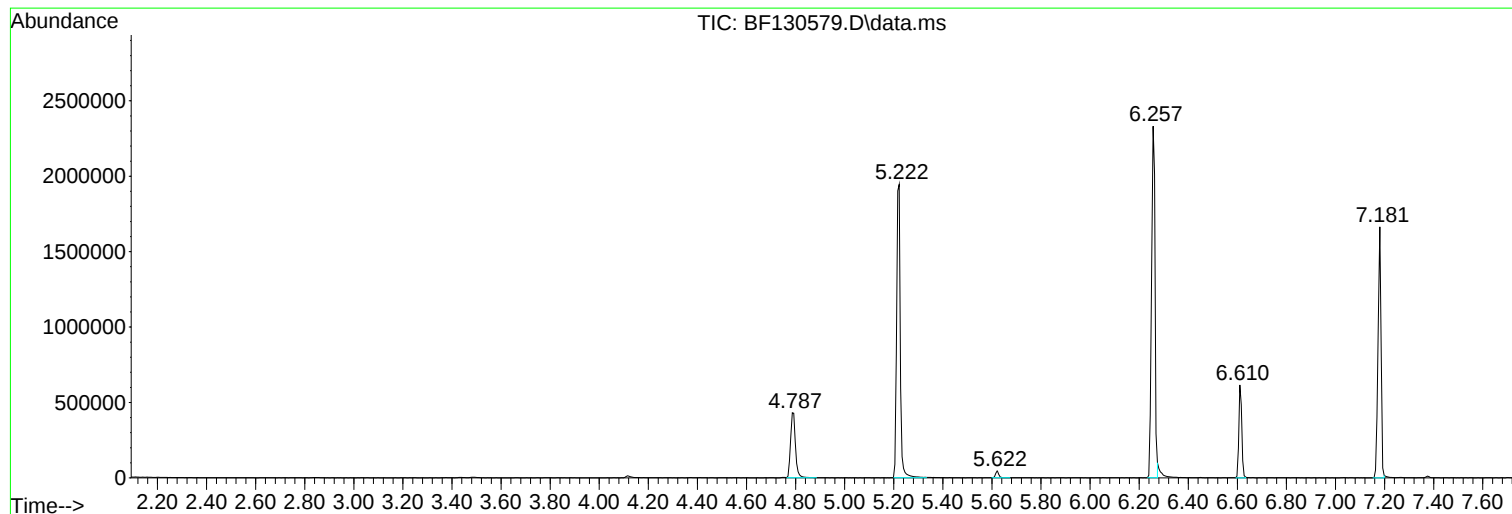

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100722\
Data File : BF130579.D
Acq On : 07 Oct 2022 17:23
Operator : CG\JU
Sample : N5046-05
Misc :
ALS Vial : 6 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
R-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
4.787	23.45 ng	595651	1,4-Dichlorobenzene-d4	6.610	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
5	(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9

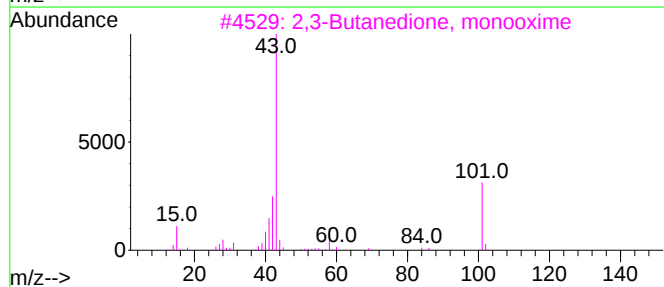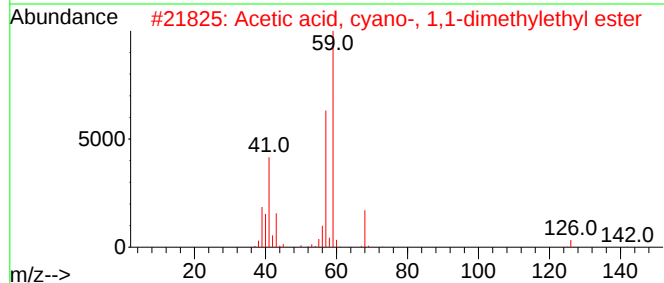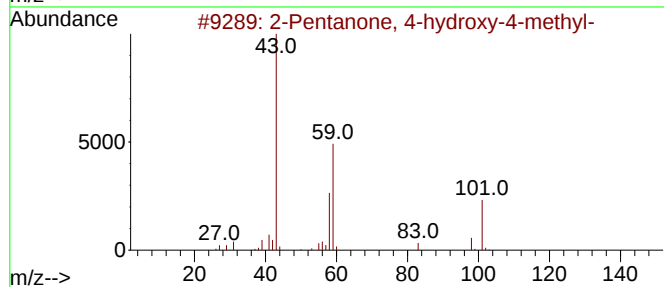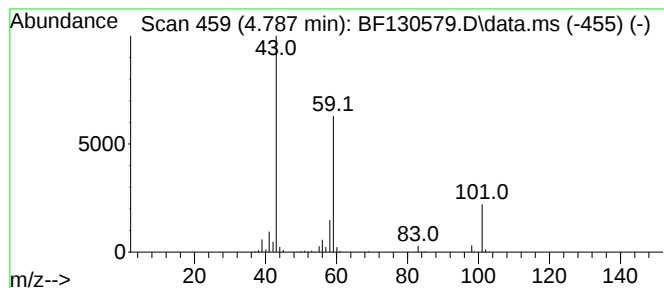

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100722\
Data File : BF130579.D
Acq On : 07 Oct 2022 17:23
Operator : CG\JU
Sample : N5046-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
R-5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.787	23.4	ng	595651	1	6.610	508054	20.0