

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100722\
 Data File : BF130588.D
 Acq On : 07 Oct 2022 22:30
 Operator : CG\JU
 Sample : N5046-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 R-12

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130588.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.775	453	457	472	rVB	304973	363056	30.67%	3.924%
2	5.210	528	531	554	rBV	1218697	1165621	98.45%	12.599%
3	5.616	597	600	606	rBV	23837	21555	1.82%	0.233%
4	6.257	705	709	729	rBV	1202052	1104966	93.33%	11.943%
5	6.610	766	769	773	rBV	495922	394153	33.29%	4.260%
6	7.181	862	866	869	rBV	790439	692474	58.49%	7.485%
7	7.893	984	987	991	rBV	601584	465564	39.32%	5.032%
8	8.969	1166	1170	1173	rBV	1635204	1183919	100.00%	12.796%
9	9.639	1281	1284	1288	rBV	553136	447865	37.83%	4.841%
10	10.428	1414	1418	1432	rBV	769856	653304	55.18%	7.061%
11	11.122	1532	1536	1539	rBV	534673	414144	34.98%	4.476%
12	12.328	1737	1741	1745	rBV	24472	23215	1.96%	0.251%
13	12.557	1775	1780	1783	rBV	31637	28462	2.40%	0.308%
14	12.704	1801	1805	1809	rBV	1381864	1160372	98.01%	12.542%
15	13.751	1979	1983	1986	rBV	615210	541899	45.77%	5.857%
16	13.774	1986	1987	1991	rVB	26378	22318	1.89%	0.241%
17	14.527	2112	2115	2118	rBV2	19423	19766	1.67%	0.214%
18	14.751	2150	2153	2156	rBV2	21971	30158	2.55%	0.326%
19	14.827	2163	2166	2169	rBV2	22840	26725	2.26%	0.289%
20	15.080	2206	2209	2214	rVB	21546	21605	1.82%	0.234%
21	15.133	2214	2218	2222	rBV	405562	448218	37.86%	4.845%
22	15.551	2286	2289	2292	rVB2	21487	22635	1.91%	0.245%




Sum of corrected areas: 9251994

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100722\
Data File : BF130588.D
Acq On : 07 Oct 2022 22:30
Operator : CG\JU
Sample : N5046-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
R-12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

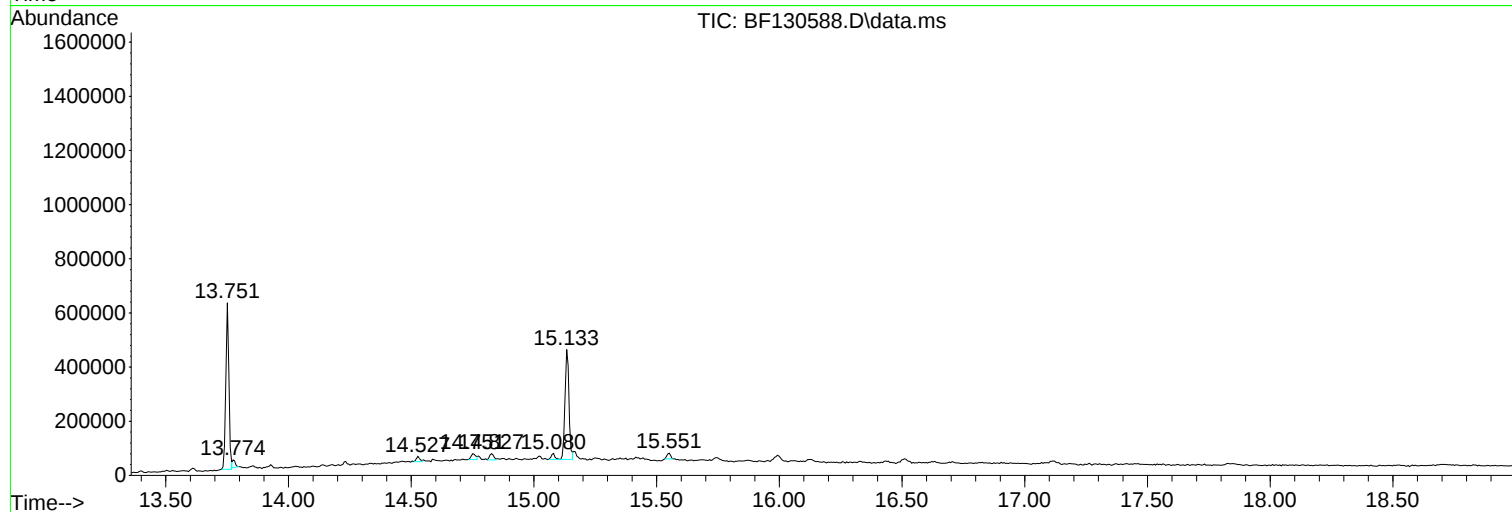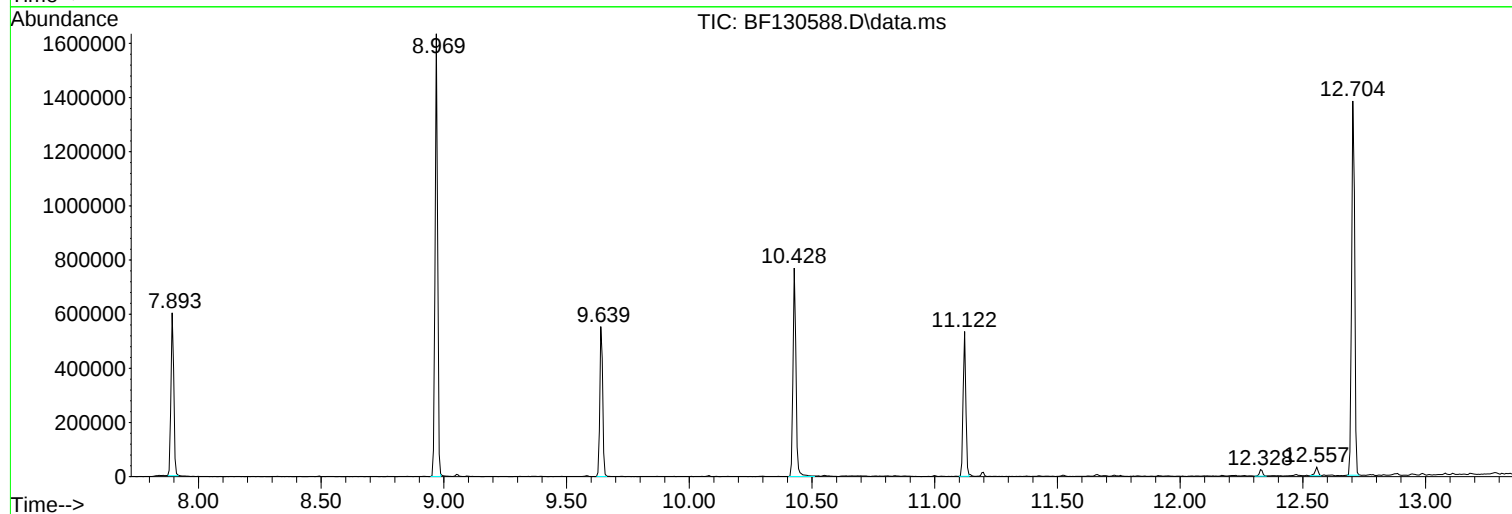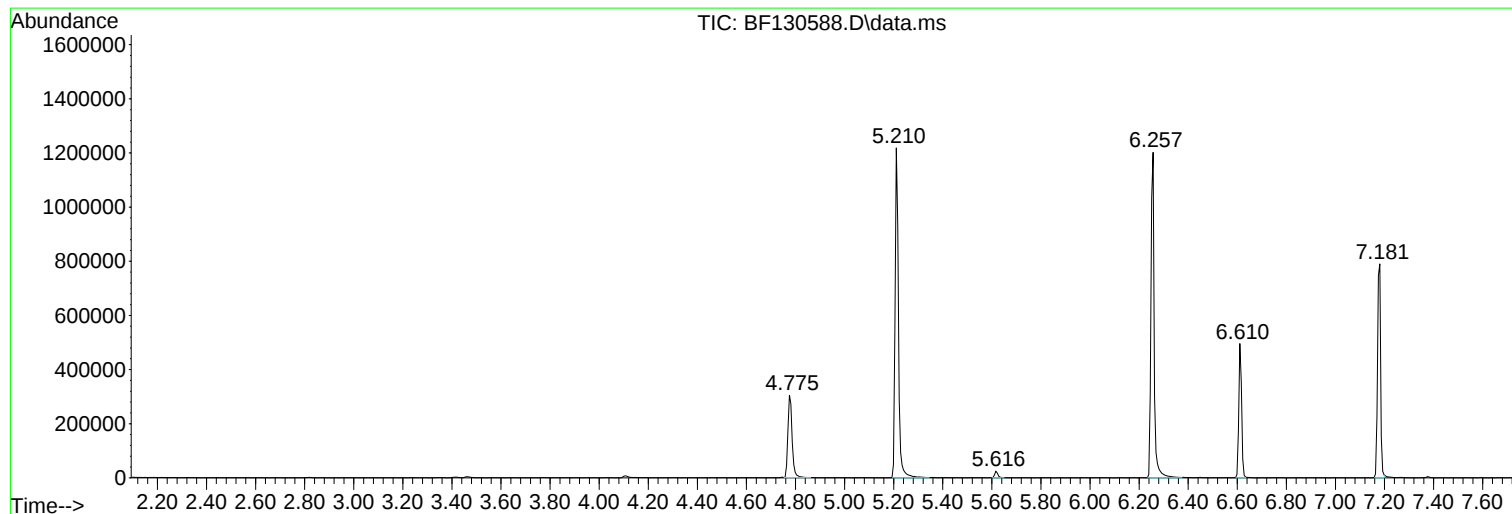

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100722\
Data File : BF130588.D
Acq On : 07 Oct 2022 22:30
Operator : CG\JU
Sample : N5046-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
R-12










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.775	18.42 ng	363056	1,4-Dichlorobenzene-d4	6.610

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25		
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		

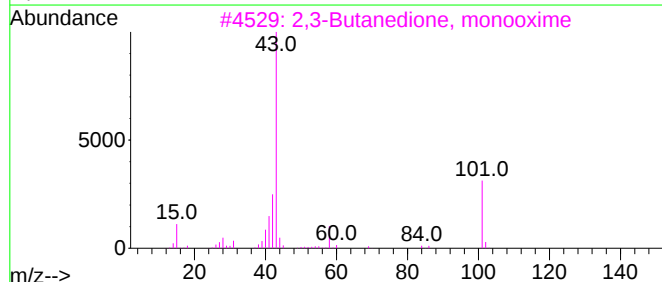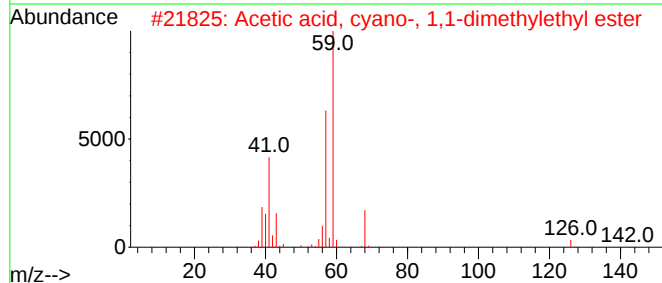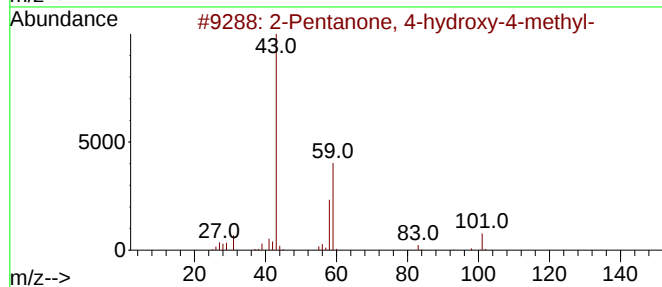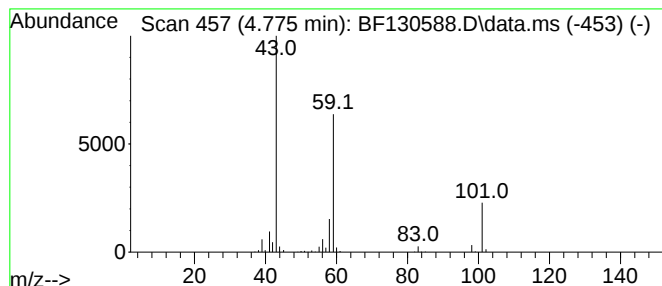

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100722\
Data File : BF130588.D
Acq On : 07 Oct 2022 22:30
Operator : CG\JU
Sample : N5046-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
R-12

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.775	18.4	ng	363056	1	6.610	394153	20.0