


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100722\
 Data File : BF130574.D
 Acq On : 07 Oct 2022 14:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 10 13:41:25 2022

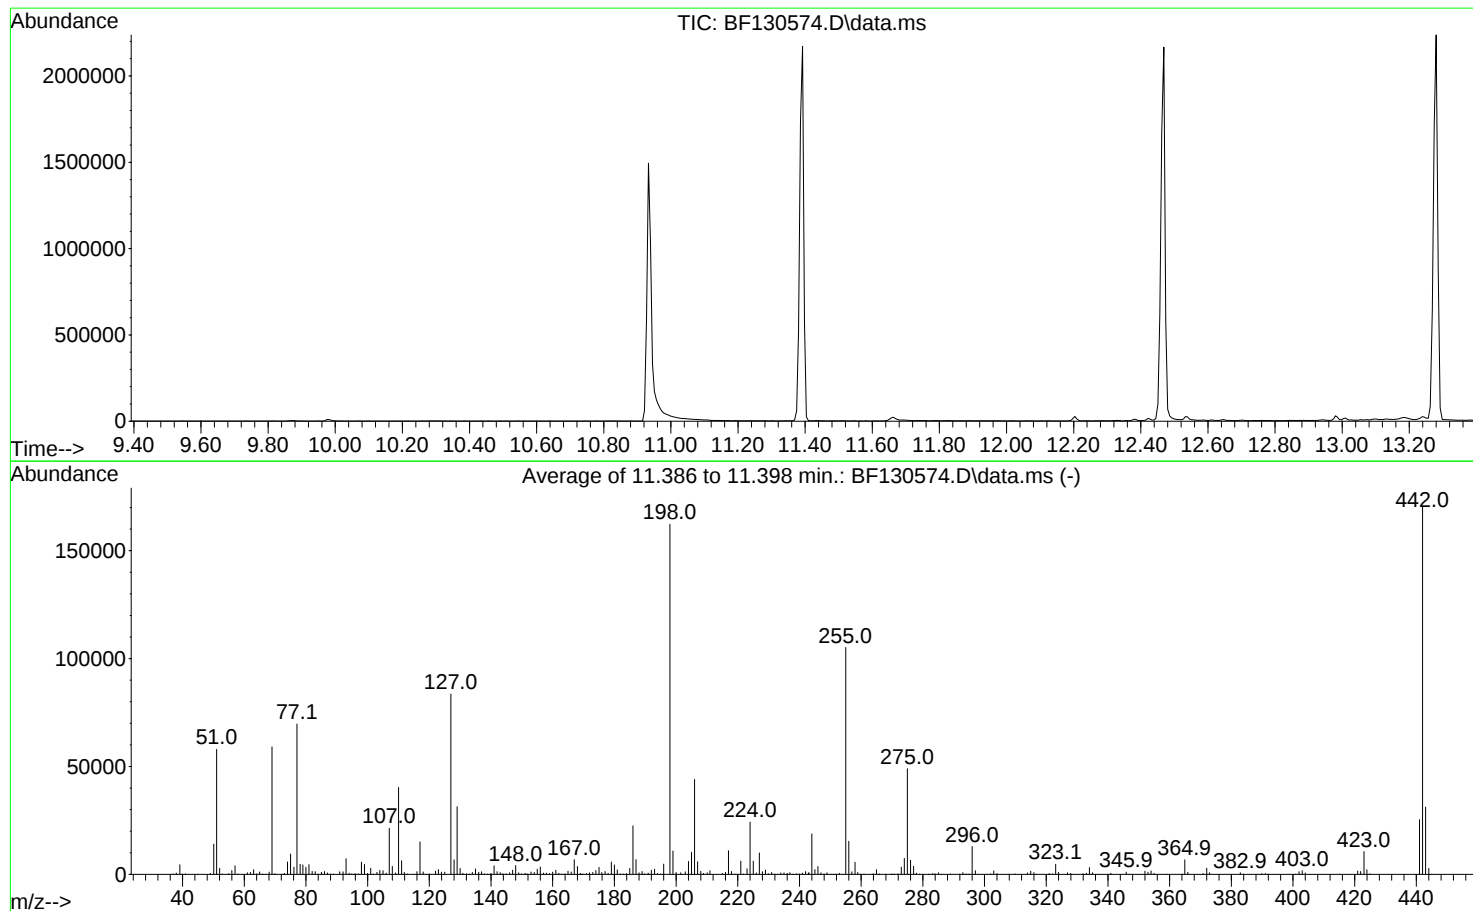




AutoFind: Scans 1581, 1582, 1583; Background Corrected with Scan 1575

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	57924	PASS
68	69	0.00	2	1.8	1057	PASS
69	198	0.00	100	36.4	59131	PASS
70	69	0.00	2	0.5	314	PASS
127	198	10	80	51.5	83560	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	162285	PASS
199	198	5	9	6.7	10813	PASS
275	198	10	60	30.1	48912	PASS
365	198	1	100	4.1	6733	PASS
441	198	0.01	100	15.6	25384	PASS
442	442	50	100	100.0	170496	PASS
443	442	15	24	18.3	31160	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100722\
 Data File : BF130574.D
 Acq On : 07 Oct 2022 14:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 10 04:11:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 07 02:06:46 2022
 Response via : Initial Calibration

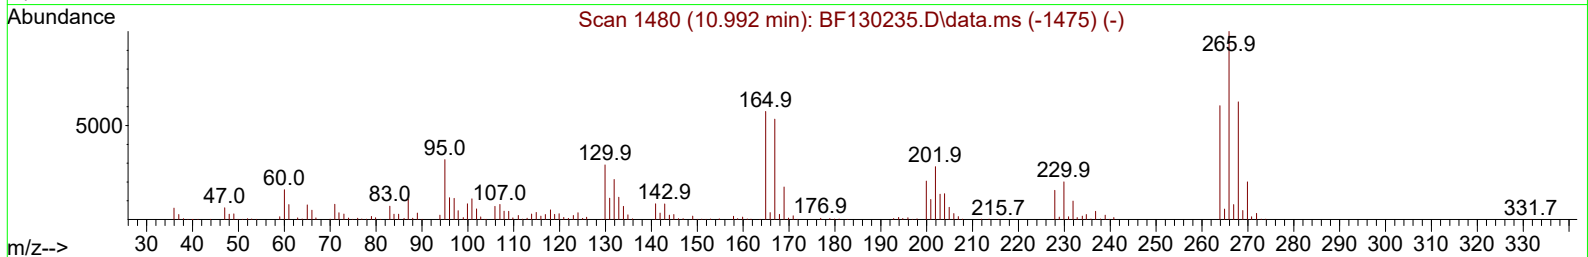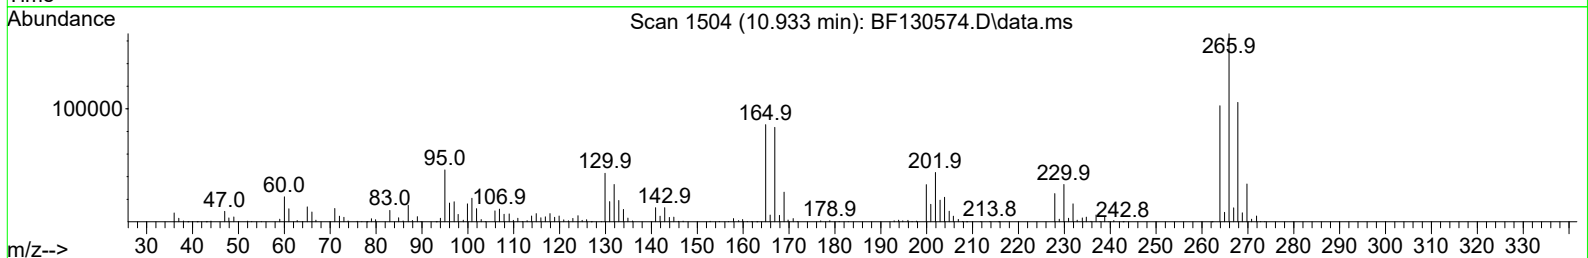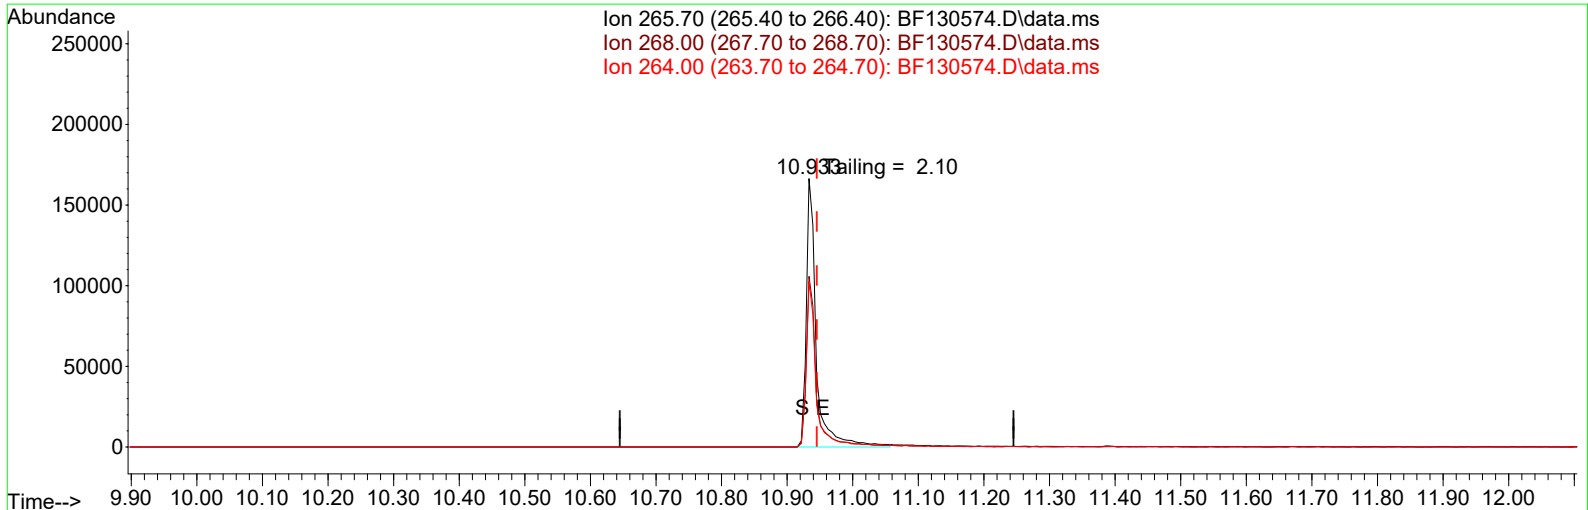

TIC: BF130574.D\data.ms

(70) Pentachlorophenol (C)

10.933min (-0.012) 456180.00 ng




response 180633

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.54
264.00	63.10	61.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100722\
Data File : BF130574.D
Acq On : 07 Oct 2022 14:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 10 04:11:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 07 02:06:46 2022
Response via : Initial Calibration

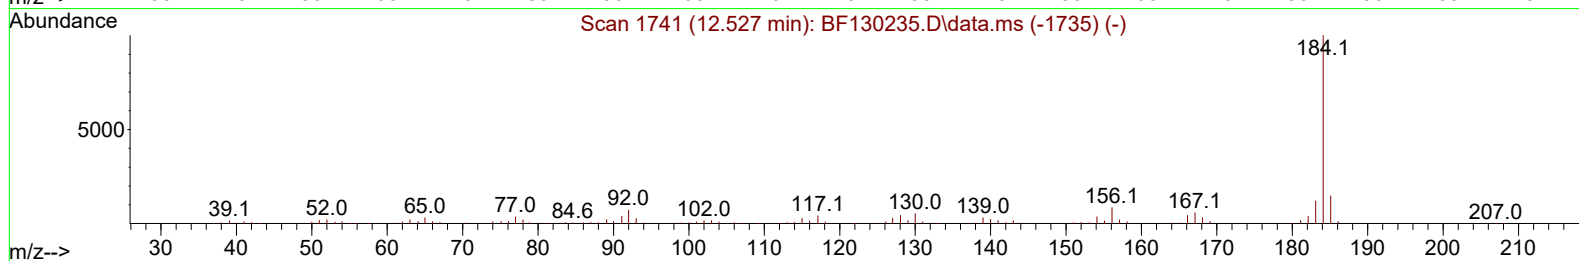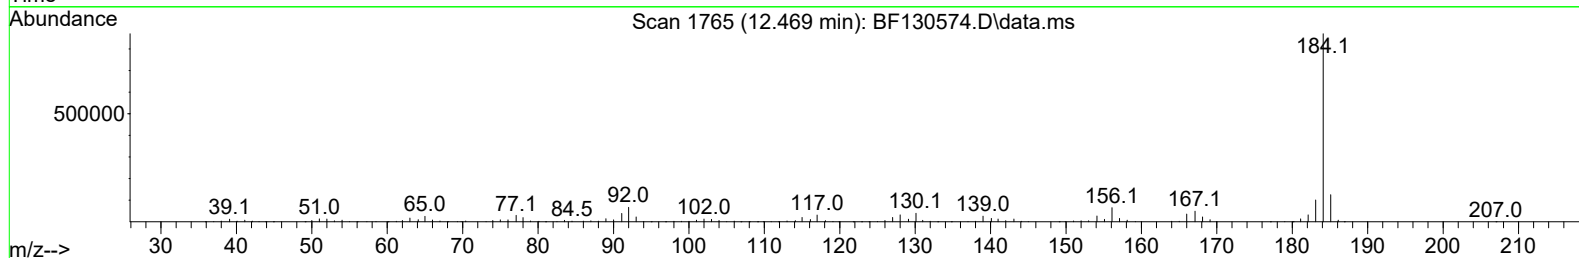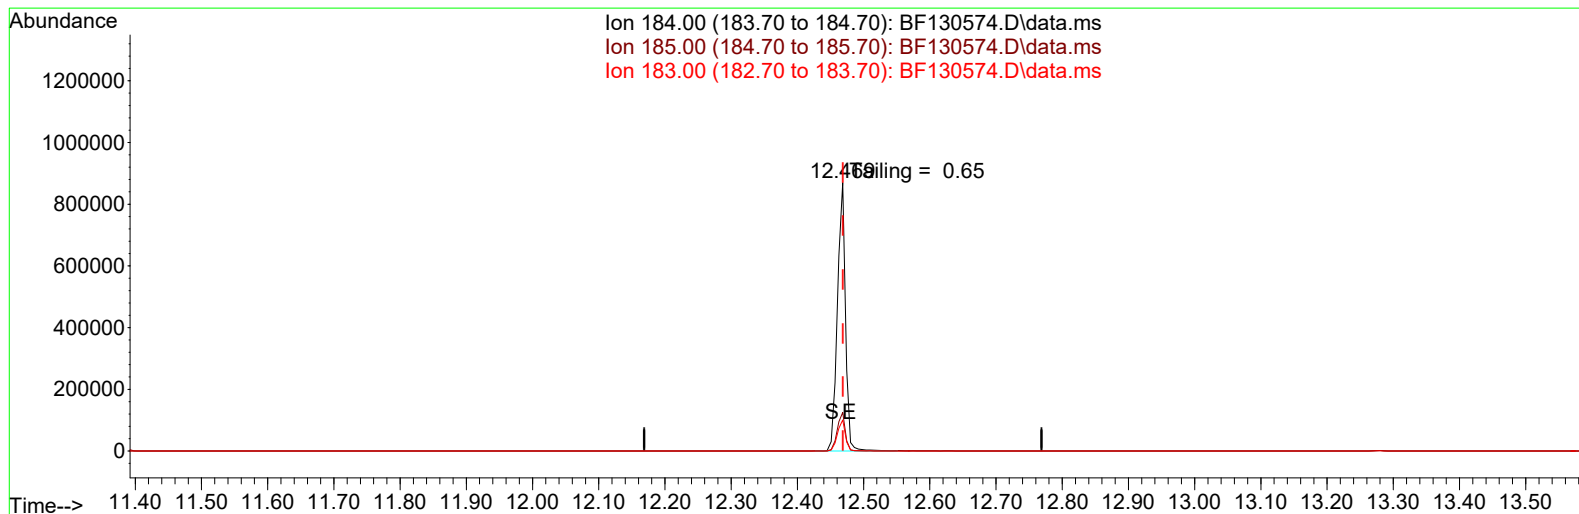

TIC: BF130574.D\data.ms

(77) Benzidine

12.469min (-0.000) 113184.94 ng

response 739273

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.40
183.00	11.40	11.61
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/7/2022	BNA_F	<u>BF130574.D</u>
Compound Name	Response	Retention Time
DDT	375624	13.28
DDD	6786	12.98
DDE	918	12.645
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7704	383328	2.01

Instrument :
BNA_F
ClientSampleId :
DFTPP