
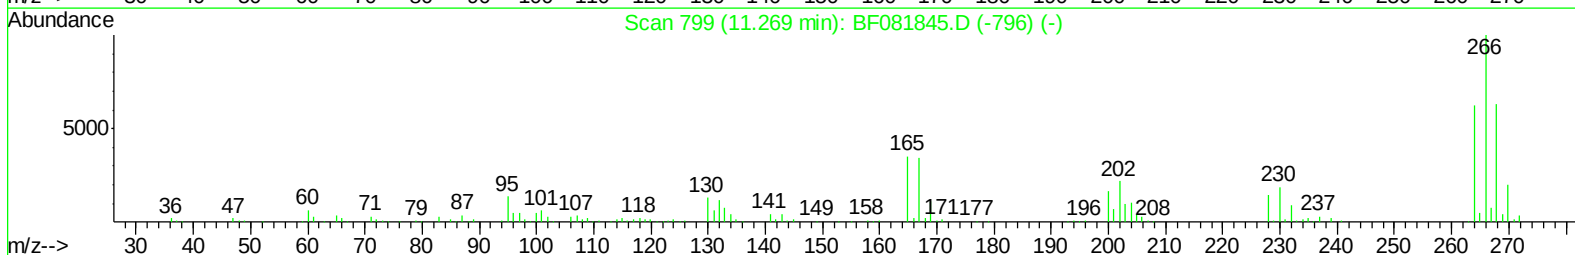
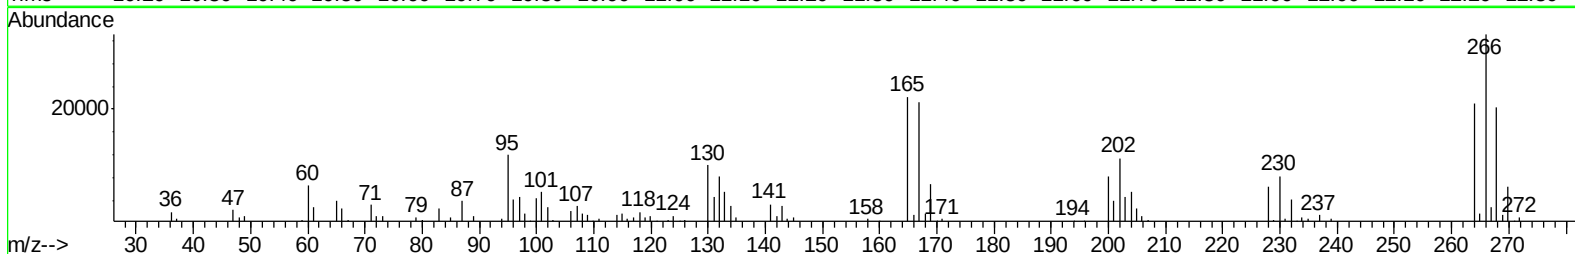


Data Path : Z:\HPCHEM1\BNA F\Data\BF100815\
Data File : BF082121.D
Acq On : 8 Oct 2015 8:31
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 09:05:19 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 08 02:46:05 2015
Response via : Initial Calibration

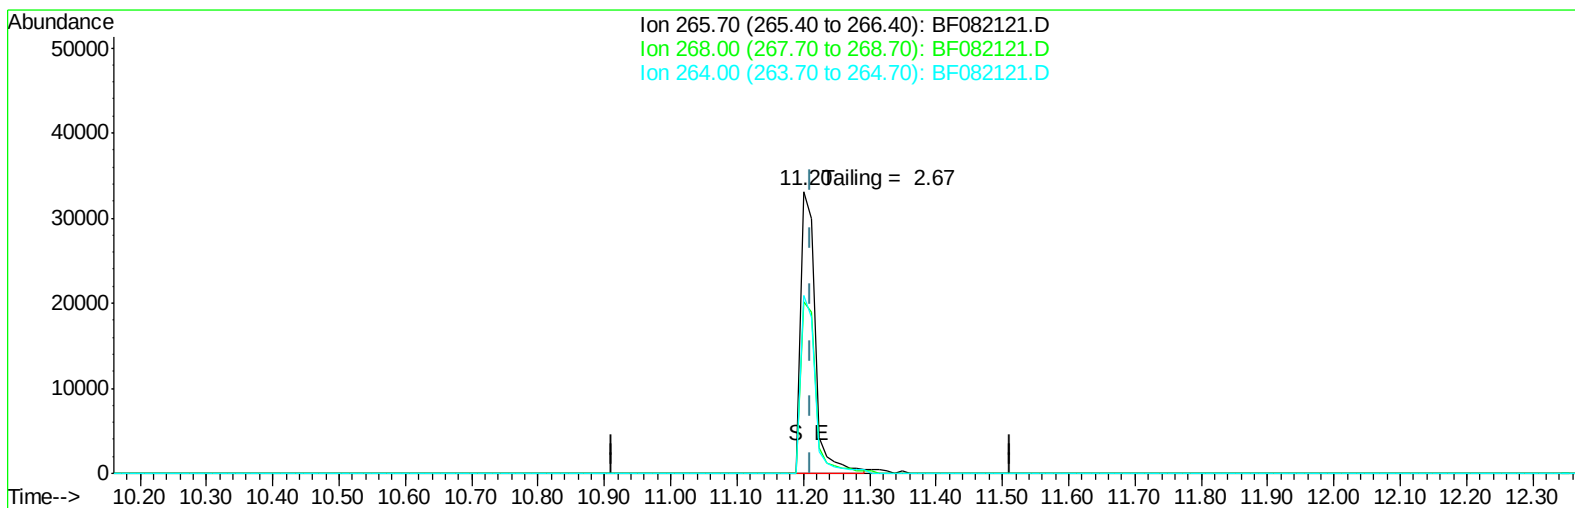

TIC: BF082121.D

(69) Pentachlorophenol (C)




11.200min (-0.012) 0.00ng

response 51350

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	61.15
264.00	62.70	63.23
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF100815\
Data File : BF082121.D
Acq On : 8 Oct 2015 8:31
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 09:05:19 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 08 02:46:05 2015
Response via : Initial Calibration

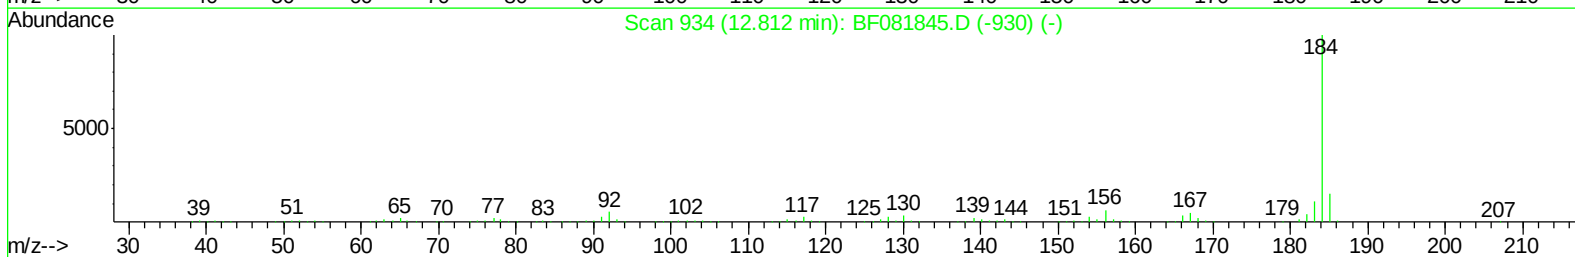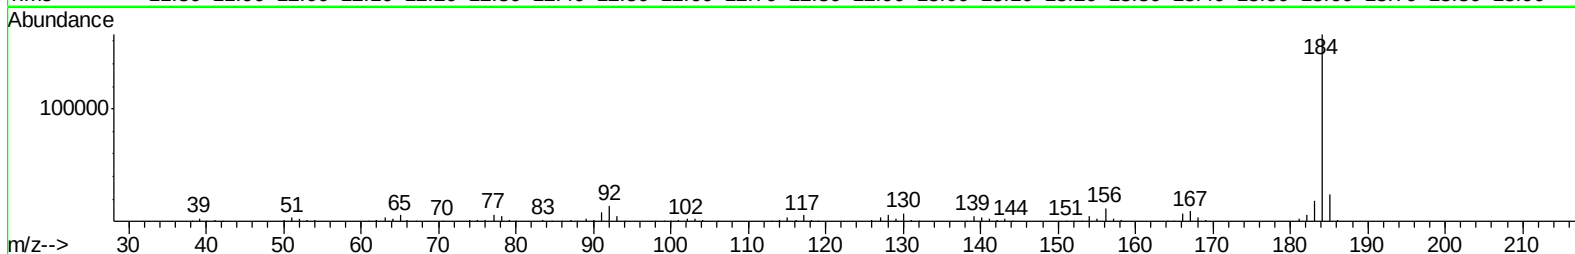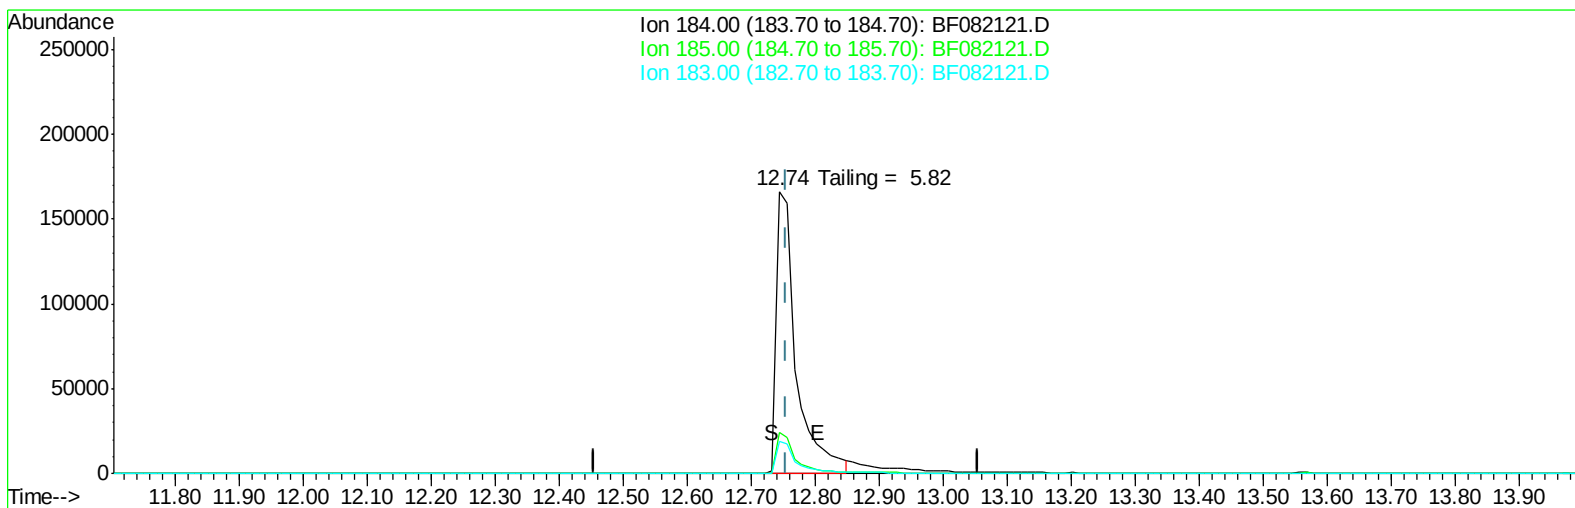

TIC: BF082121.D

(76) Benzidine

12.743min (-0.012) 11733.76ng

response 378640

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.36
183.00	9.50	11.23
0.00	0.00	0.00