

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100815\
 Data File : BF082137.D
 Acq On : 8 Oct 2015 20:10
 Operator : UM/IZ
 Sample : G3960-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-2

Quant Time: Oct 09 08:58:32 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 09 05:03:35 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	73137	20.00	ng	-0.01
21) Naphthalene-d8	8.15	136	305506	20.00	ng	0.00
38) Acenaphthene-d10	9.90	164	145552	20.00	ng	-0.01
63) Phenanthrene-d10	11.39	188	293729	20.00	ng	0.00
75) Chrysene-d12	14.02	240	282867	20.00	ng	-0.02
86) Perylene-d12	15.48	264	210908	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.45	112	272106	67.54	ng	0.00
7) Phenol-d6	6.49	99	206916	40.81	ng	0.00
23) Nitrobenzene-d5	7.43	82	448304	97.82	ng	-0.01
41) 2,4,6-Tribromophenol	10.70	330	226942	153.95	ng	0.00
44) 2-Fluorobiphenyl	9.22	172	894734	108.66	ng	-0.01
78) Terphenyl-d14	12.98	244	1031713	144.87	ng	0.00
Target Compounds						
2) 1,4-Dioxane	2.46	88	99331	56.69	ng	Qvalue 88
49) Dimethylphthalate	9.62	163	58369	5.81	ng	# 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100815\
Data File : BF082137.D
Acq On : 8 Oct 2015 20:10
Operator : UM/IZ
Sample : G3960-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-2

Quant Time: Oct 09 08:58:32 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 09 05:03:35 2015
Response via : Initial Calibration

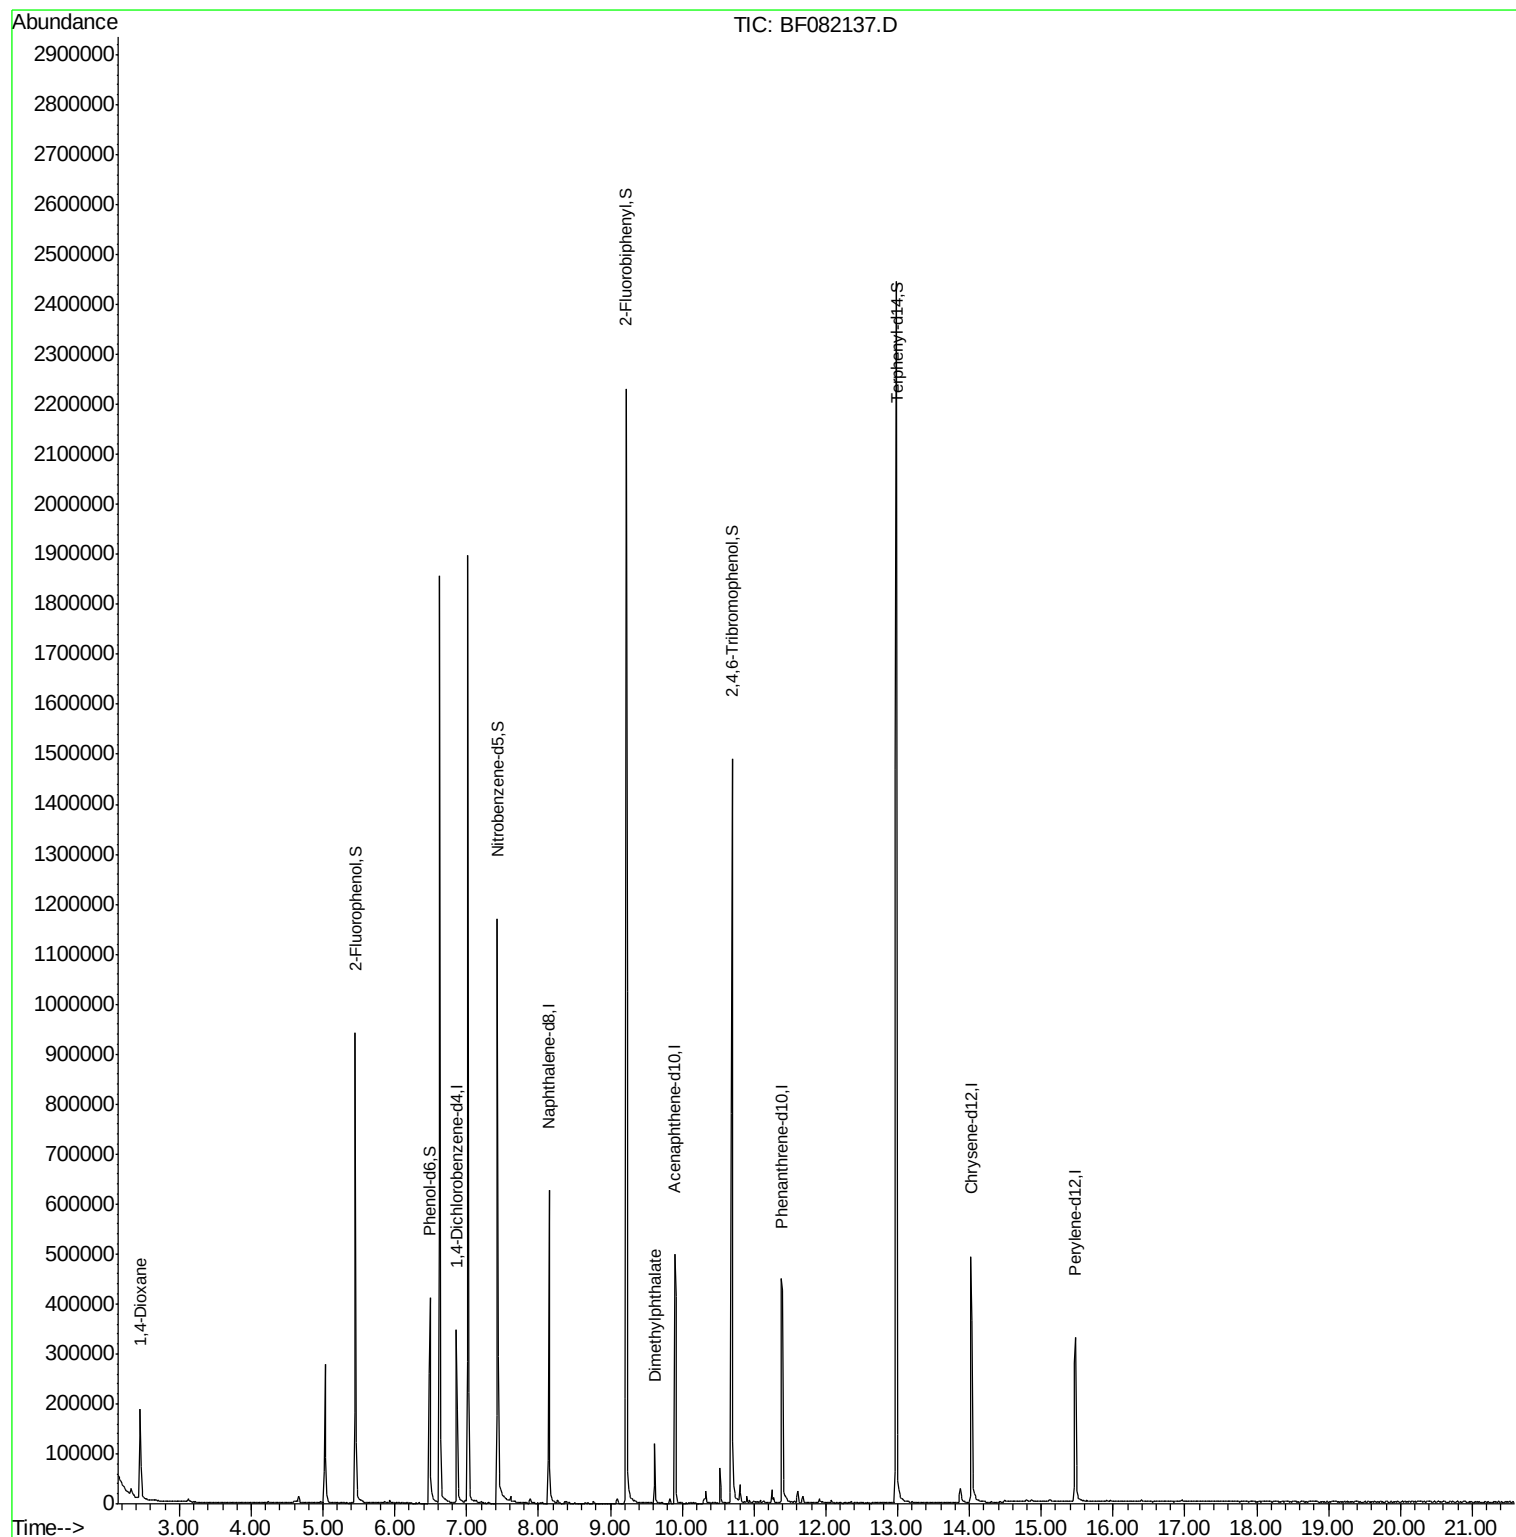

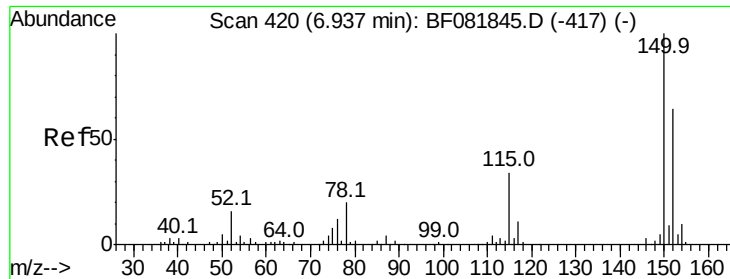

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.86 min Scan# 413

Delta R.T. -0.01 min

Lab File: BF082137.D

Acq: 8 Oct 2015 20:10

Instrument :

BNA_F

ClientSampleId :

MW-2


Tot Ion:152 Resp: 73137

Ion Ratio Lower Upper

152 100

150 161.9 124.7 187.1




115 62.8 39.0 58.4#

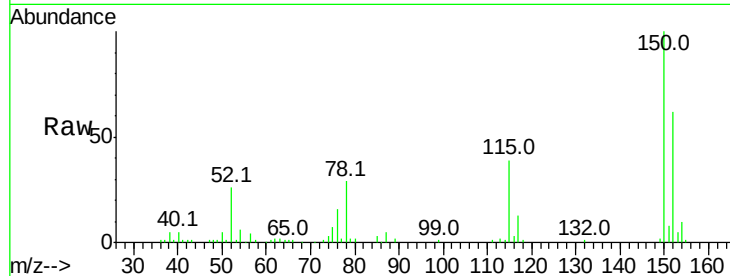

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

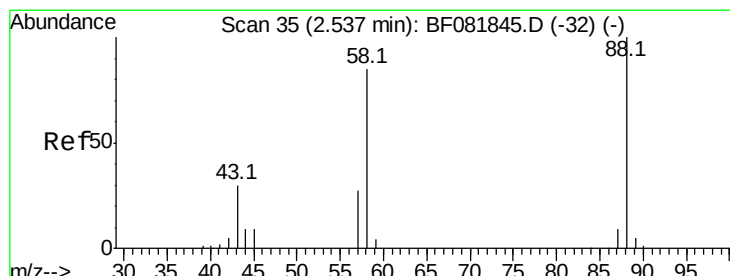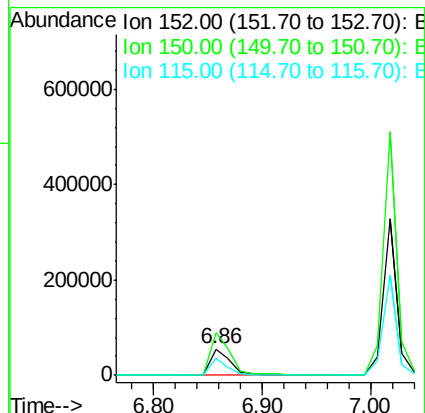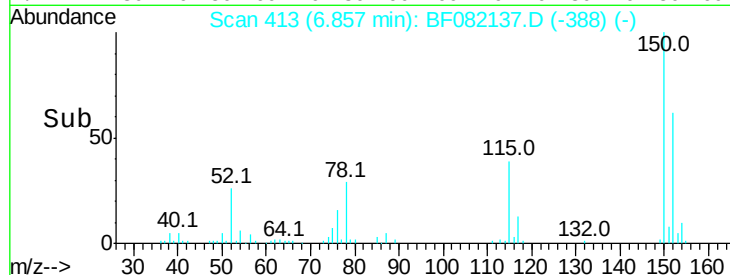

#2

1,4-Dioxane

Concen: 56.69 ng

RT: 2.46 min Scan# 28

Delta R.T. 0.03 min

Lab File: BF082137.D

Acq: 8 Oct 2015 20:10


Tgt Ion: 88 Resp: 99331

Ion Ratio Lower Upper

88 100

58 83.5 77.7 116.5



43 29.8 26.6 40.0

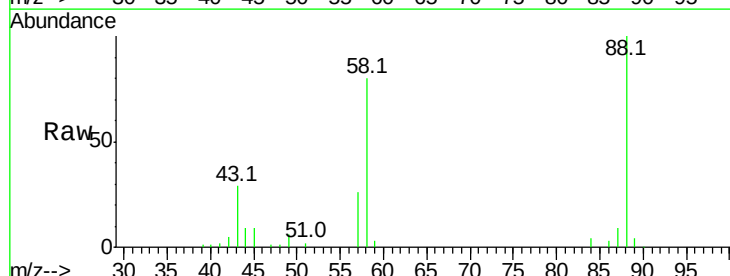


Abundance Ion 88.00 (87.70 to 88.70): BF0

Ion 58.00 (57.70 to 58.70): BF0

Ion 43.00 (42.70 to 43.70): BF0

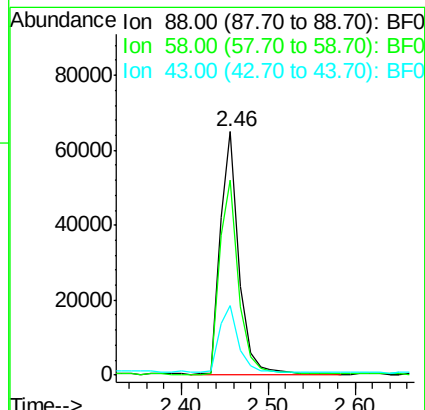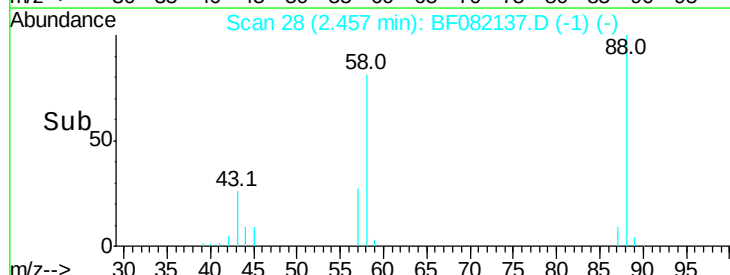

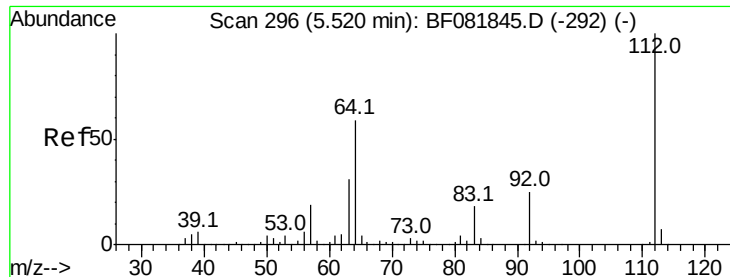

#5

2-Fluorophenol

Concen: 67.54 ng

RT: 5.45 min Scan# 290

Delta R.T. -0.00 min

Lab File: BF082137.D

Acq: 8 Oct 2015 20:10

Instrument :

BNA_F

ClientSampleId :

MW-2


Tot Ion:112 Resp: 272106

Ion Ratio Lower Upper

112 100

64 58.7 39.7 59.5




63 30.9 17.4 26.0#

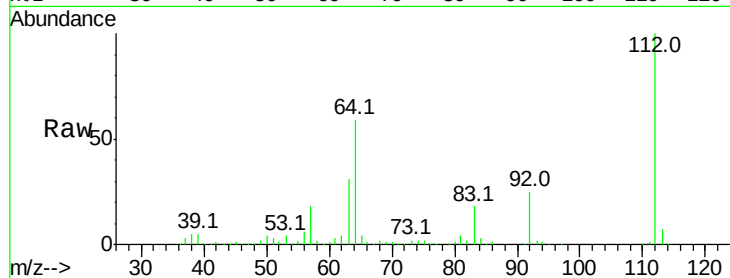

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

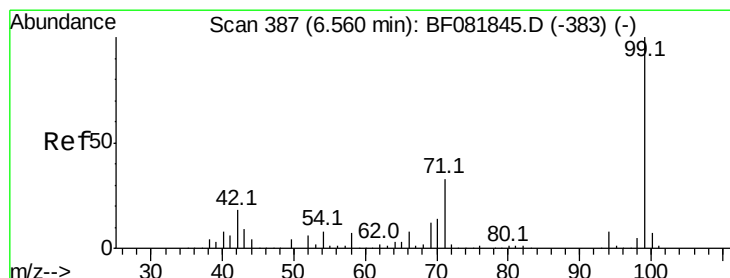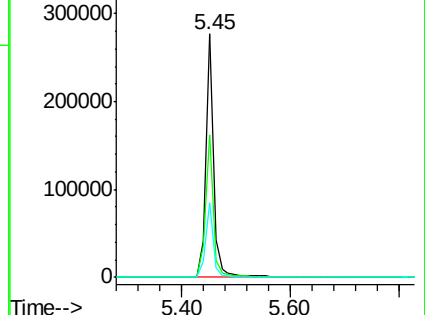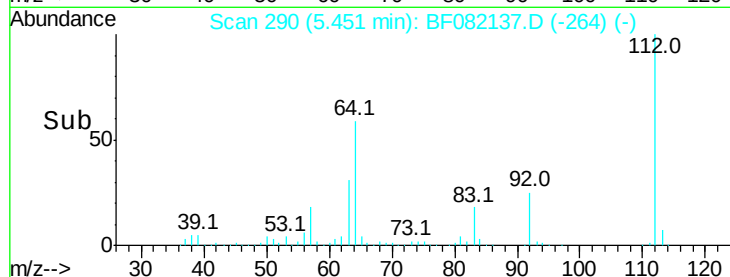

#7

Phenol-d6

Concen: 40.81 ng

RT: 6.49 min Scan# 381

Delta R.T. -0.00 min

Lab File: BF082137.D

Acq: 8 Oct 2015 20:10


Tgt Ion: 99 Resp: 206916

Ion Ratio Lower Upper

99 100

42 13.5 13.7 20.5#



71 29.0 14.2 21.2#

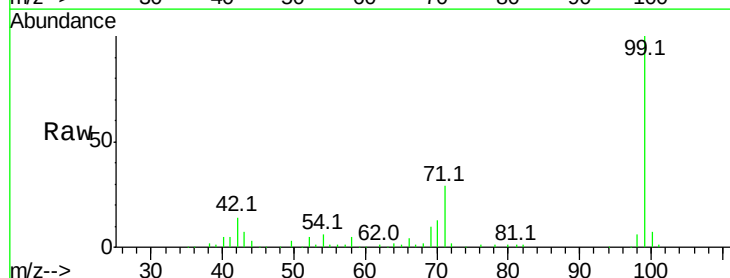


Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0



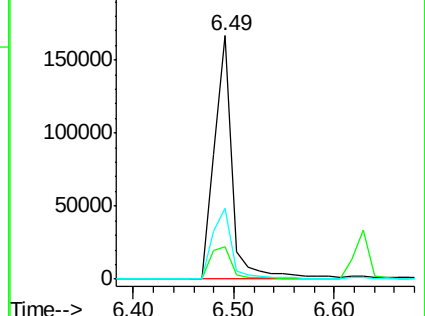
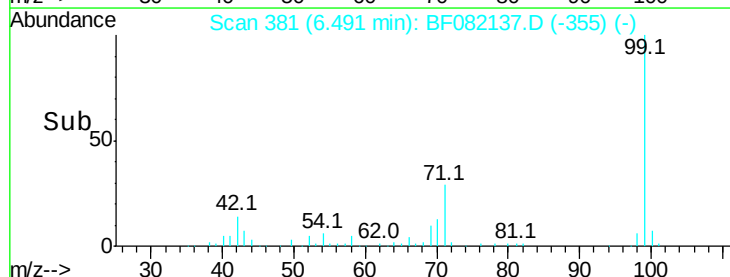


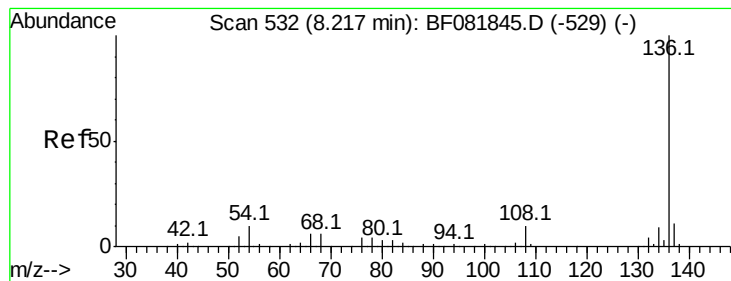

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.15 min Scan# 526
Delta R.T. -0.00 min
Lab File: BF082137.D
Acq: 8 Oct 2015 20:10




Instrument :
BNA_F
ClientSampleID :
MW-2


Tot Ion:	136	Resp:	305506
Ion	Ratio	Lower	Upper
136	100		
137	11.0	9.0	13.6
54	7.7	8.2	12.2#
68	5.0	5.8	8.6#

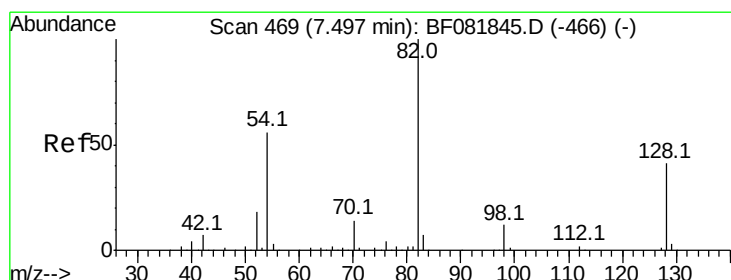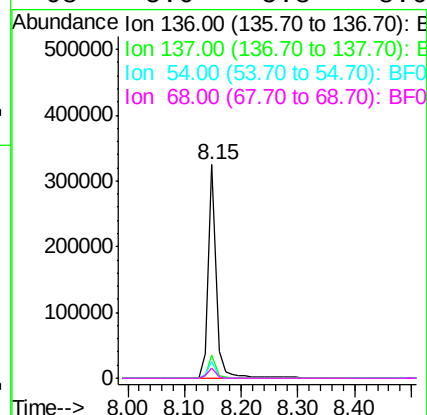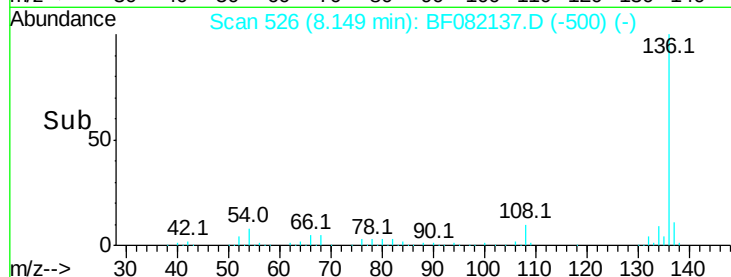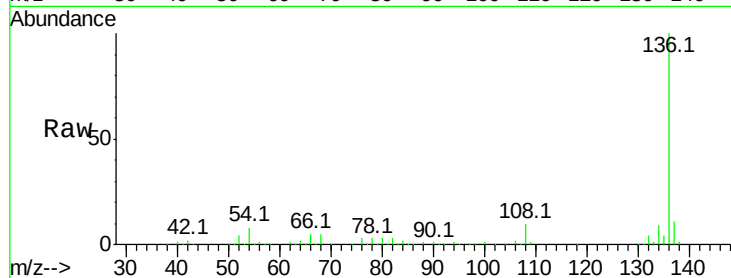

#23
Nitrobenzene-d5
Concen: 97.82 ng
RT: 7.43 min Scan# 463
Delta R.T. -0.01 min
Lab File: BF082137.D
Acq: 8 Oct 2015 20:10

Tgt Ion:	82	Resp:	448304
Ion	Ratio	Lower	Upper
82	100		
128	42.4	51.0	76.6#
54	55.5	47.5	71.3

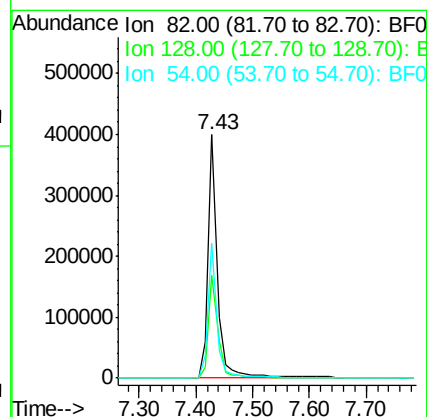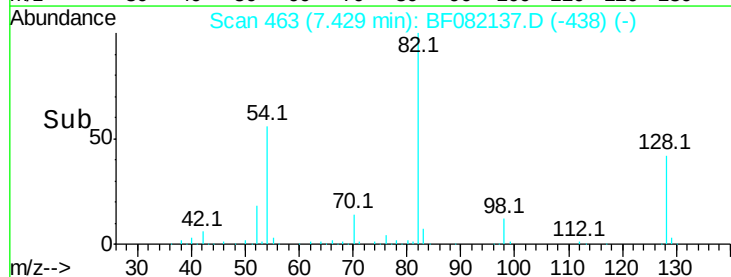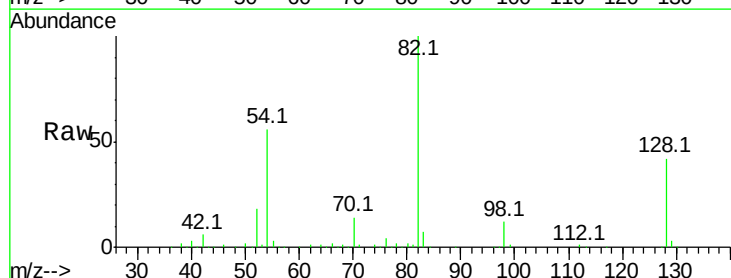


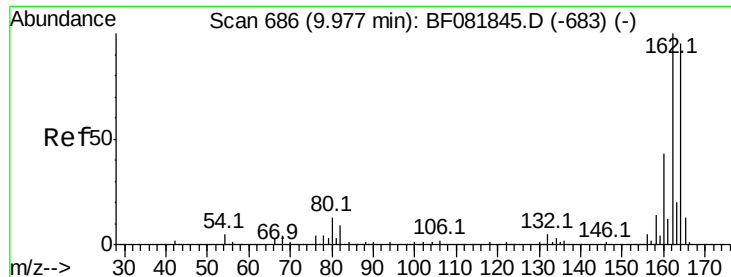




#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.90 min Scan# 679
Delta R.T. -0.01 min
Lab File: BF082137.D
Acq: 8 Oct 2015 20:10

Instrument :
BNA_F
ClientSampleId :
MW-2

Tot Ion:164 Resp: 145552
Ion Ratio Lower Upper
164 100
162 103.2 75.2 112.8
160 44.4 31.5 47.3

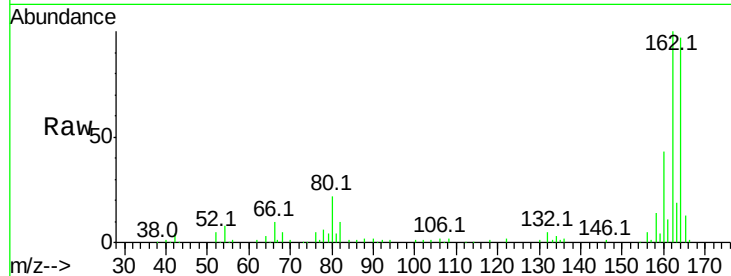


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

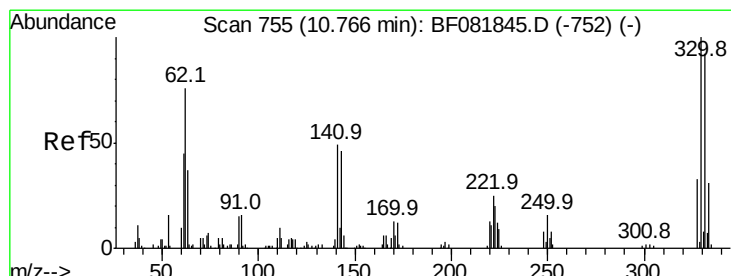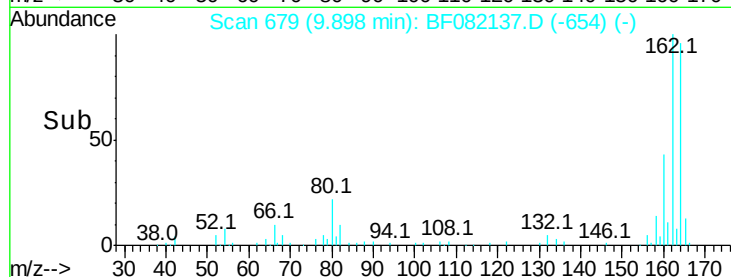
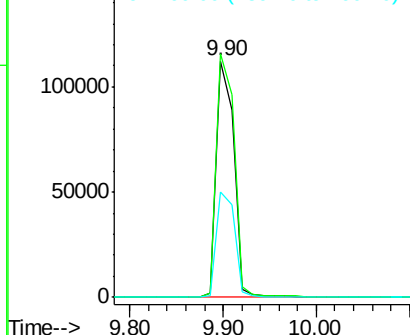



#41
2,4,6-Tribromophenol
Concen: 153.95 ng
RT: 10.70 min Scan# 749
Delta R.T. -0.00 min
Lab File: BF082137.D
Acq: 8 Oct 2015 20:10

Tgt Ion:330 Resp: 226942
Ion Ratio Lower Upper
330 100
332 94.7 76.6 114.8
141 35.1 29.7 44.5

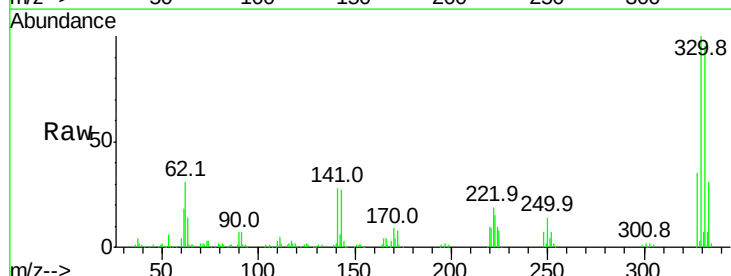

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E



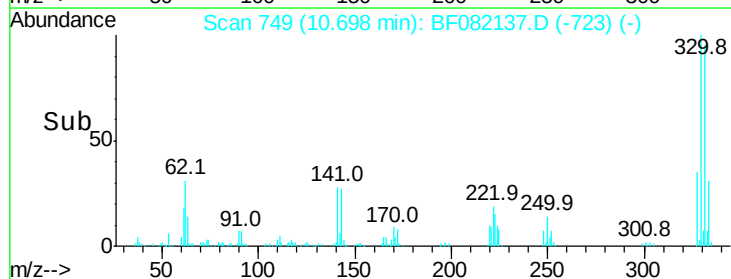
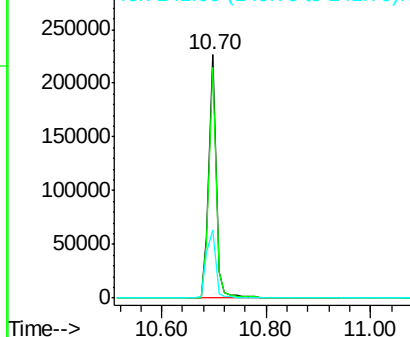


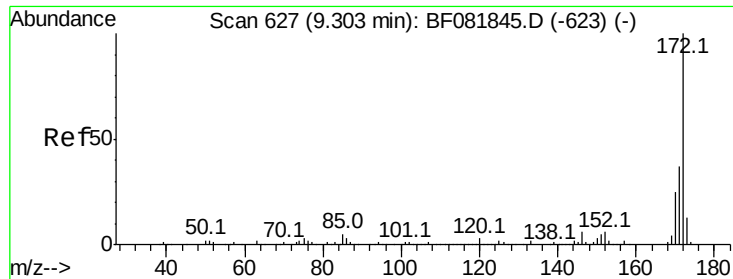

#44
 2-Fluorobiphenyl
 Concen: 108.66 ng
 RT: 9.22 min Scan# 620
 Delta R.T. -0.01 min
 Lab File: BF082137.D
 Acq: 8 Oct 2015 20:10




Instrument :
 BNA_F
 ClientSampleId :
 MW-2


Tot Ion:172 Resp: 894734
 Ion Ratio Lower Upper
 172 100
 171 35.9 26.1 39.1
 170 24.3 17.4 26.2

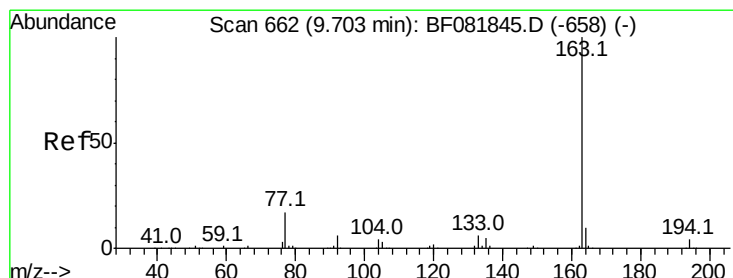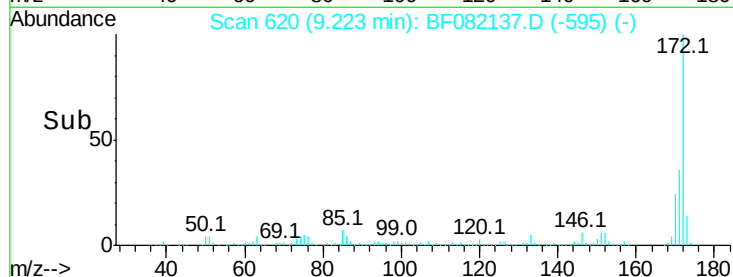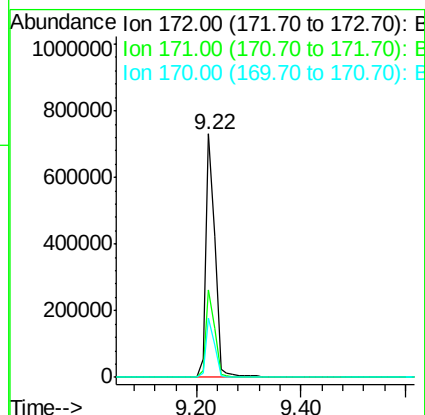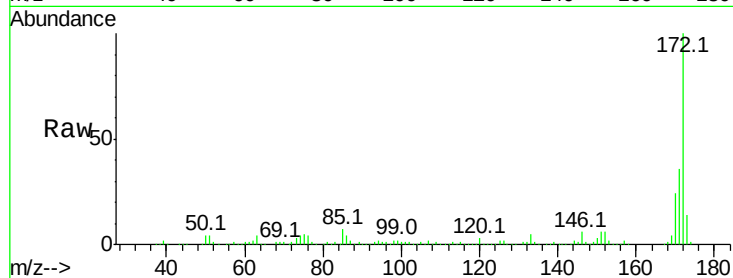

#49
 Dimethylphthalate
 Concen: 5.81 ng
 RT: 9.62 min Scan# 655
 Delta R.T. -0.01 min
 Lab File: BF082137.D
 Acq: 8 Oct 2015 20:10

Tgt Ion:163 Resp: 58369
 Ion Ratio Lower Upper
 163 100
 194 3.9 4.4 6.6#
 164 9.5 8.3 12.5


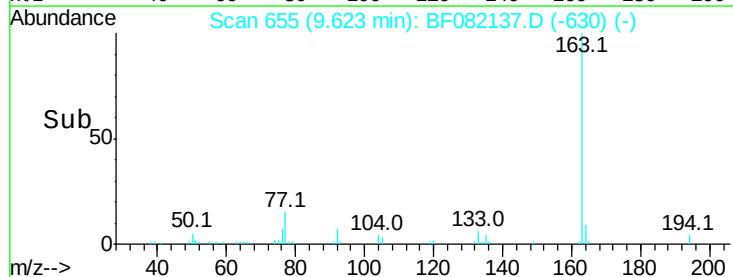
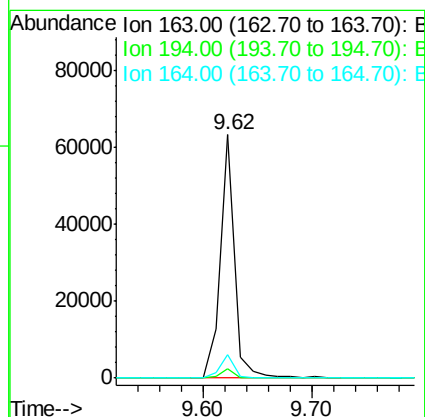
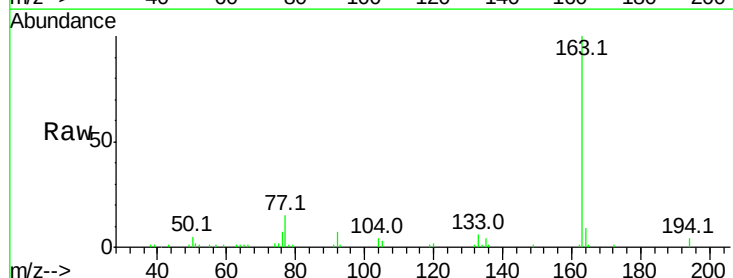


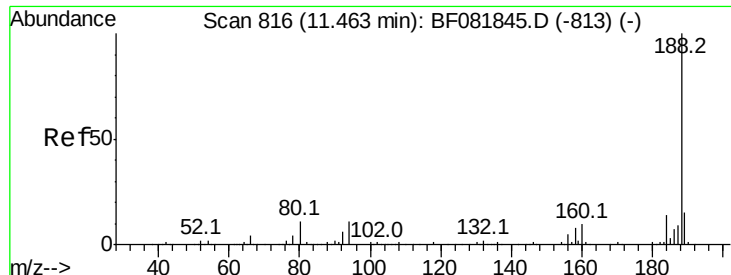

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.39 min Scan# 810
Delta R.T. -0.00 min
Lab File: BF082137.D
Acq: 8 Oct 2015 20:10




Instrument :
BNA_F
ClientSampled :
MW-2


Tot Ion:188 Resp: 293729
Ion Ratio Lower Upper
188 100
94 5.8 11.1 16.7#
80 6.0 11.0 16.4#

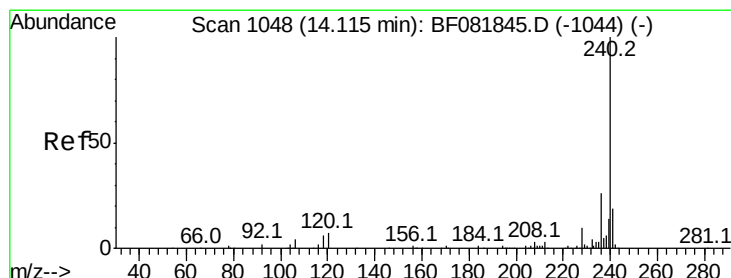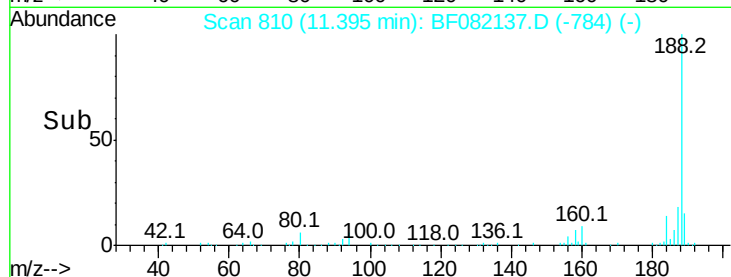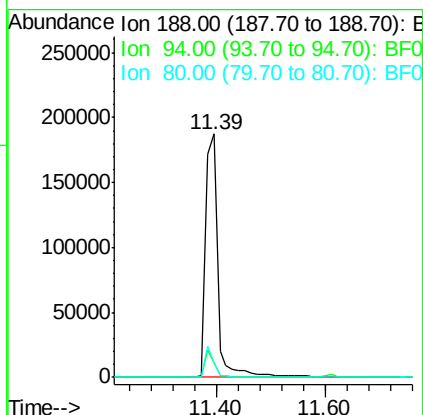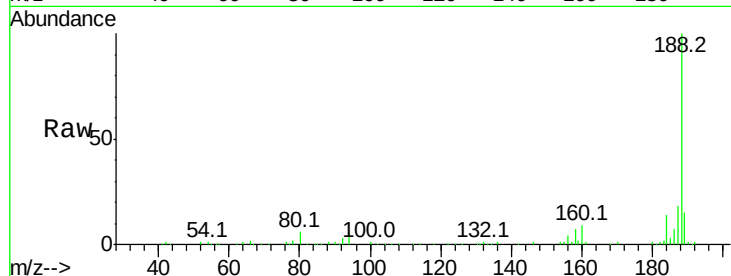

#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.02 min Scan# 1040
Delta R.T. -0.02 min
Lab File: BF082137.D
Acq: 8 Oct 2015 20:10

Tgt Ion:240 Resp: 282867
Ion Ratio Lower Upper
240 100
120 13.1 16.2 24.2#
236 25.3 18.4 27.6


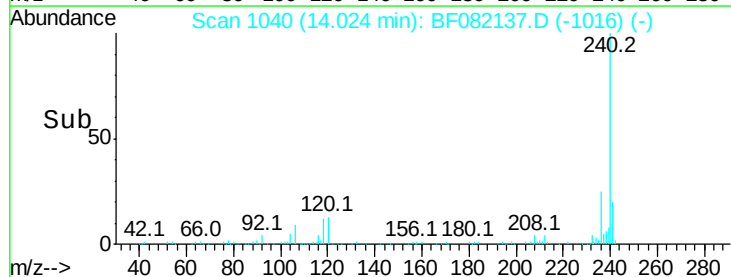
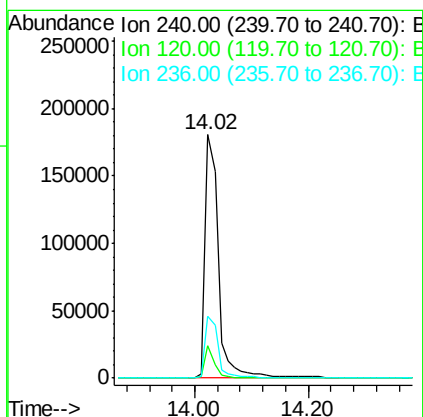
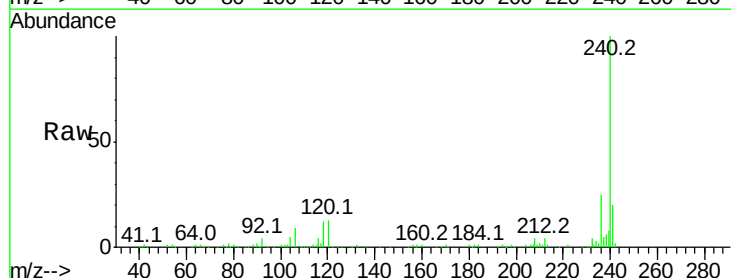


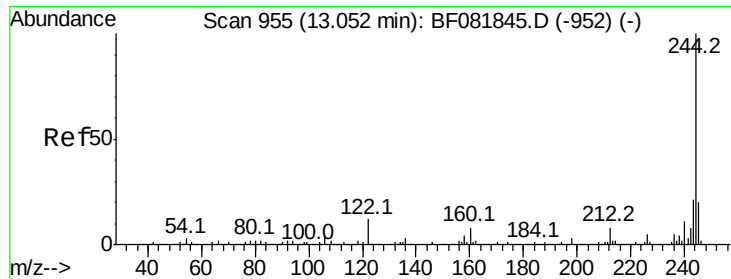

#78
 Terphenyl-d14
 Concen: 144.87 ng
 RT: 12.98 min Scan# 949
 Delta R.T. -0.00 min
 Lab File: BF082137.D
 Acq: 8 Oct 2015 20:10

Instrument :
 BNA_F
 ClientSampleId :
 MW-2

Tot Ion:244 Resp: 1031713
 Ion Ratio Lower Upper
 244 100
 212 7.1 4.3 6.5#
 122 7.7 17.4 26.2#

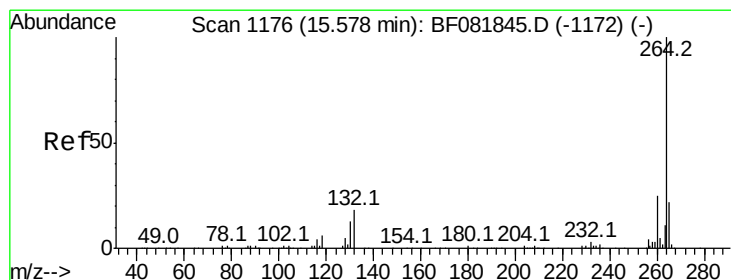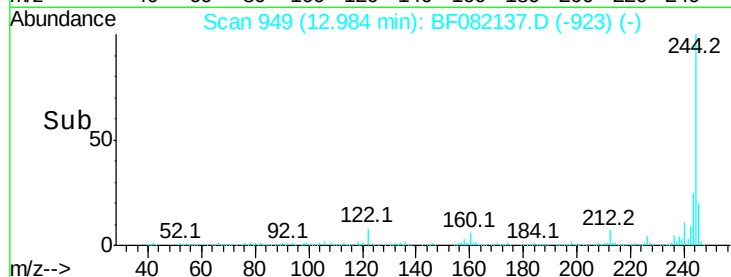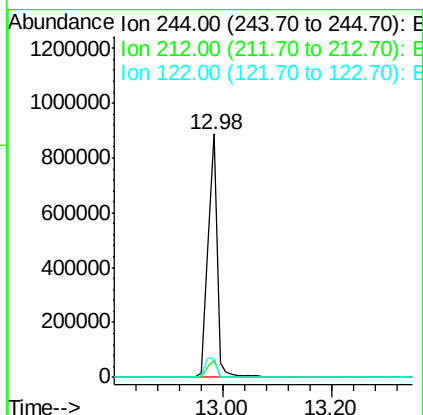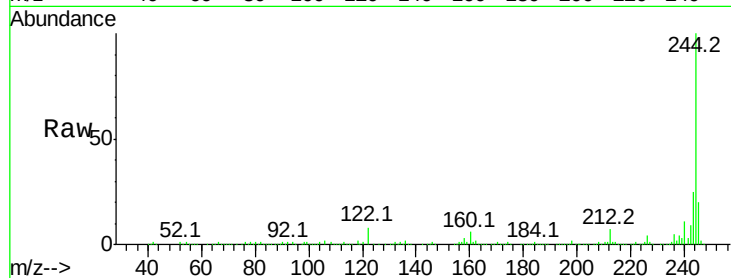

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.48 min Scan# 1167
 Delta R.T. -0.01 min
 Lab File: BF082137.D
 Acq: 8 Oct 2015 20:10

Tgt Ion:264 Resp: 210908
 Ion Ratio Lower Upper
 264 100
 260 24.5 16.7 25.1
 265 21.4 17.2 25.8

