

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100815\
 Data File : BF082126.D
 Acq On : 8 Oct 2015 14:13
 Operator : UM/IZ
 Sample : G3920-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC100515

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.400	196	198	210	rBV	474606	754638	23.03%	3.434%
2	5.051	253	255	266	rVB	404678	663058	20.24%	3.017%
3	5.463	289	291	294	rBV	1518764	1805395	55.11%	8.214%
4	6.492	378	381	384	rBV	1419454	1585148	48.38%	7.212%
5	6.629	391	393	396	rBV	2156741	2106830	64.31%	9.586%
6	6.857	411	413	416	rBV	341774	460120	14.04%	2.093%
7	7.017	425	427	430	rBV	1990172	1797181	54.86%	8.177%
8	7.429	460	463	466	rBV	1208887	1267508	38.69%	5.767%
9	8.149	523	526	528	rBV	713060	648137	19.78%	2.949%
10	9.223	618	620	623	rBV	2297183	2698468	82.37%	12.278%
11	9.623	653	655	657	rBV	41246	38292	1.17%	0.174%
12	9.898	677	679	682	rBV	536731	754986	23.05%	3.435%
13	10.698	746	749	751	rBV	1682005	1841365	56.21%	8.378%
14	11.395	807	810	812	rBV	567004	745072	22.74%	3.390%
15	12.984	946	949	951	rBV	3138051	3276127	100.00%	14.906%
16	13.875	1025	1027	1037	rBV2	17392	45656	1.39%	0.208%
17	14.035	1038	1041	1043	rBV	629554	782868	23.90%	3.562%
18	14.218	1055	1057	1059	rVB	47550	40956	1.25%	0.186%
19	15.475	1164	1167	1173	rBV	475570	666793	20.35%	3.034%


Sum of corrected areas: 21978598

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100815\
Data File : BF082126.D
Acq On : 8 Oct 2015 14:13
Operator : UM/IZ
Sample : G3920-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC100515

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

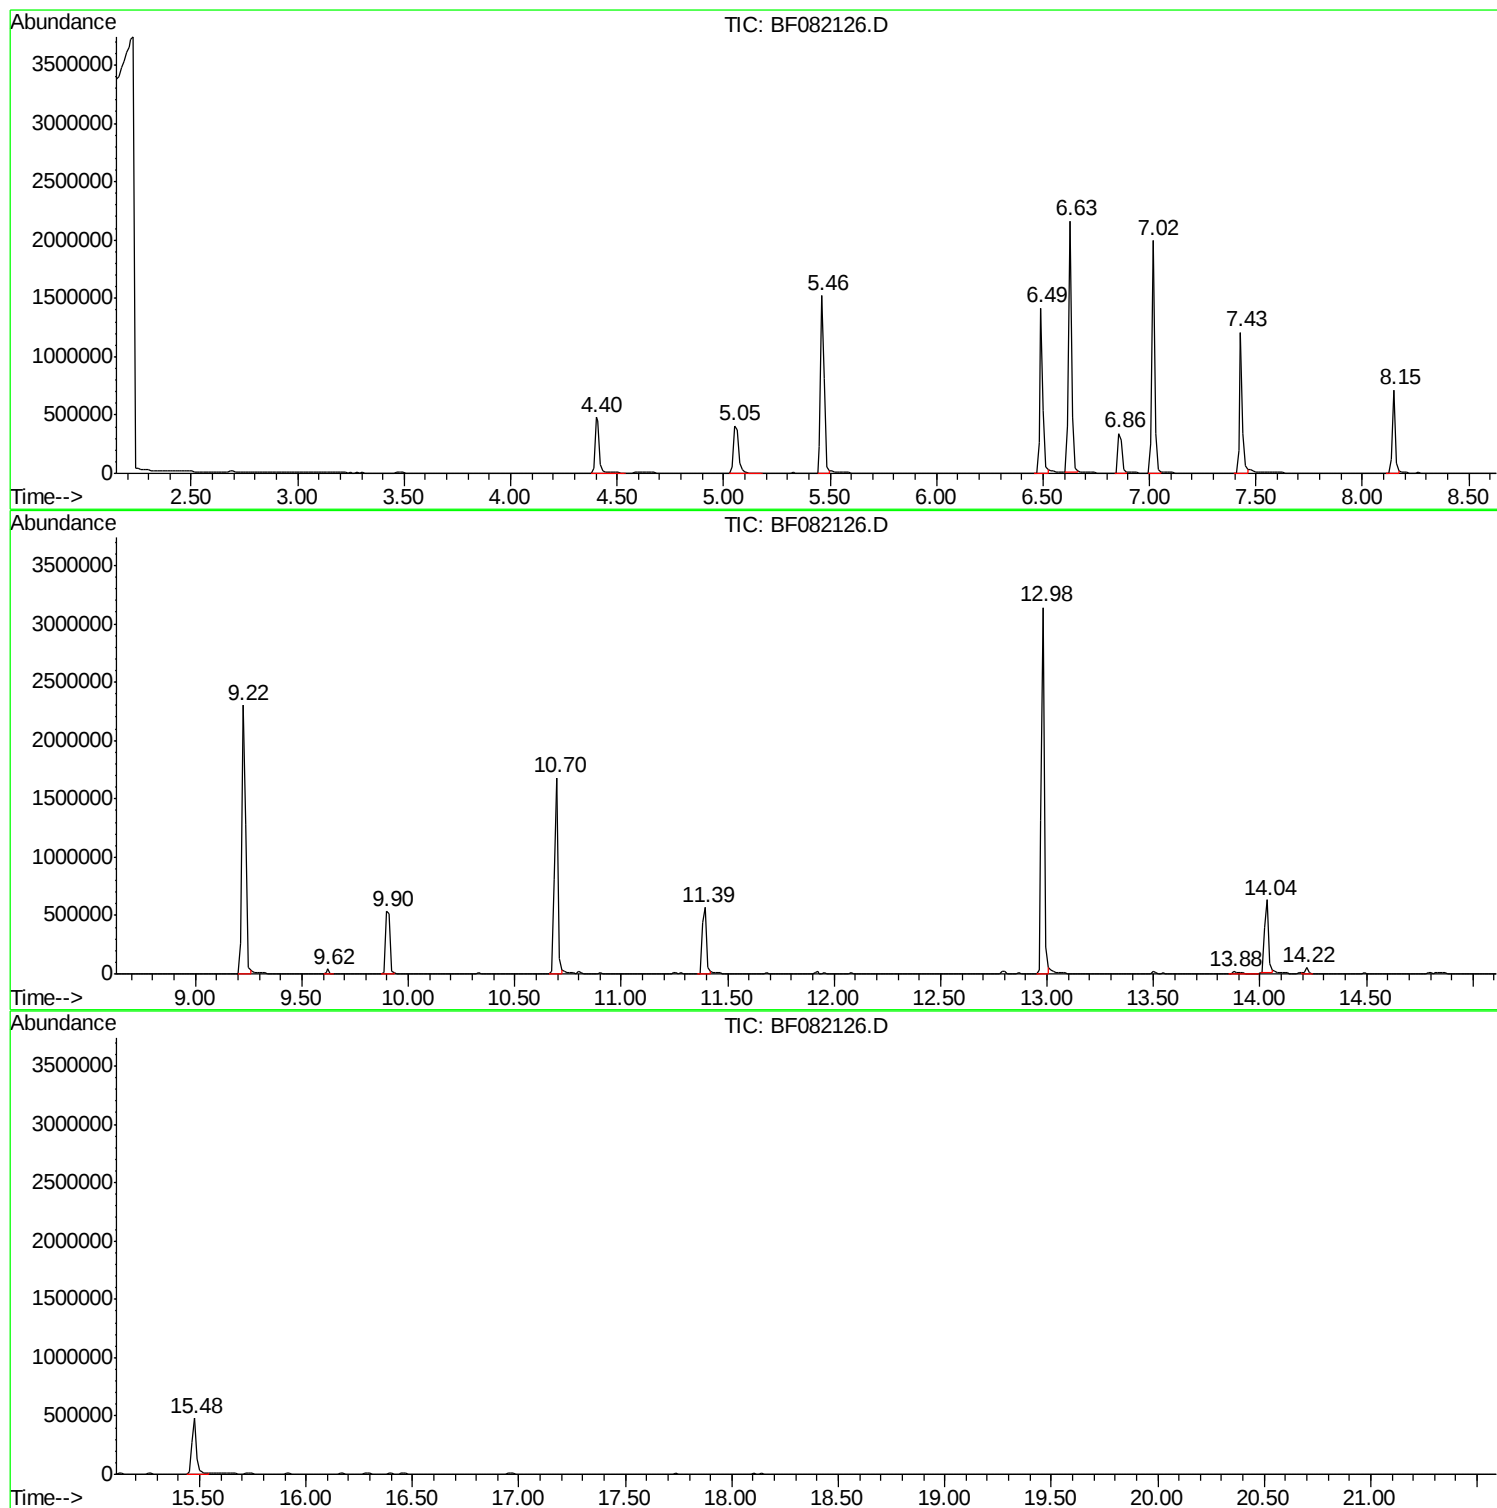

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF100815\
Data_File : BF082126.D
Acq_On : 8_Oct_2015 14:133
Operator : UM/IZZ
Sample : G3920-033
Misc :
ALS_Vial : 27 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
WC100515

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
