


Data Path : Z:\HPCHEM1\BNA F\Data\BF100815\
 Data File : BF082121.D
 Acq On : 8 Oct 2015 10:39
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 08 02:46:05 2015

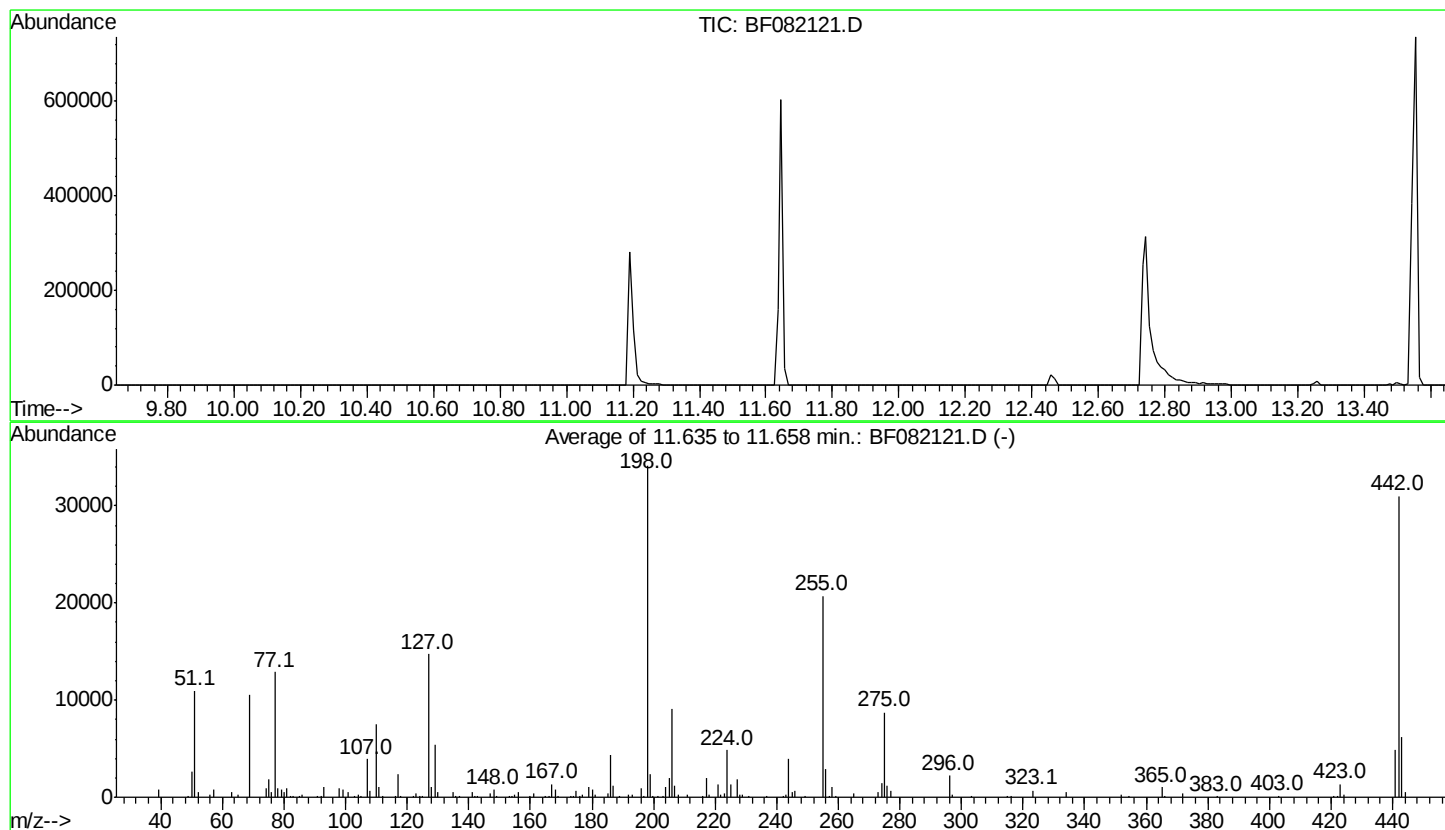

AutoFind: Scans 831, 832, 833; Background Corrected with Scan 828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.1	10969	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.7	10482	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.1	14704	PASS
197	198	0.00	2	0.4	120	PASS
198	198	100	100	100.0	34137	PASS
199	198	5	9	6.9	2341	PASS
275	198	10	60	25.5	8721	PASS
365	198	1	100	2.9	1002	PASS
441	442	0.01	24	15.6	4828	PASS
442	198	50	100	90.9	31016	PASS
443	442	15	24	19.8	6148	PASS