
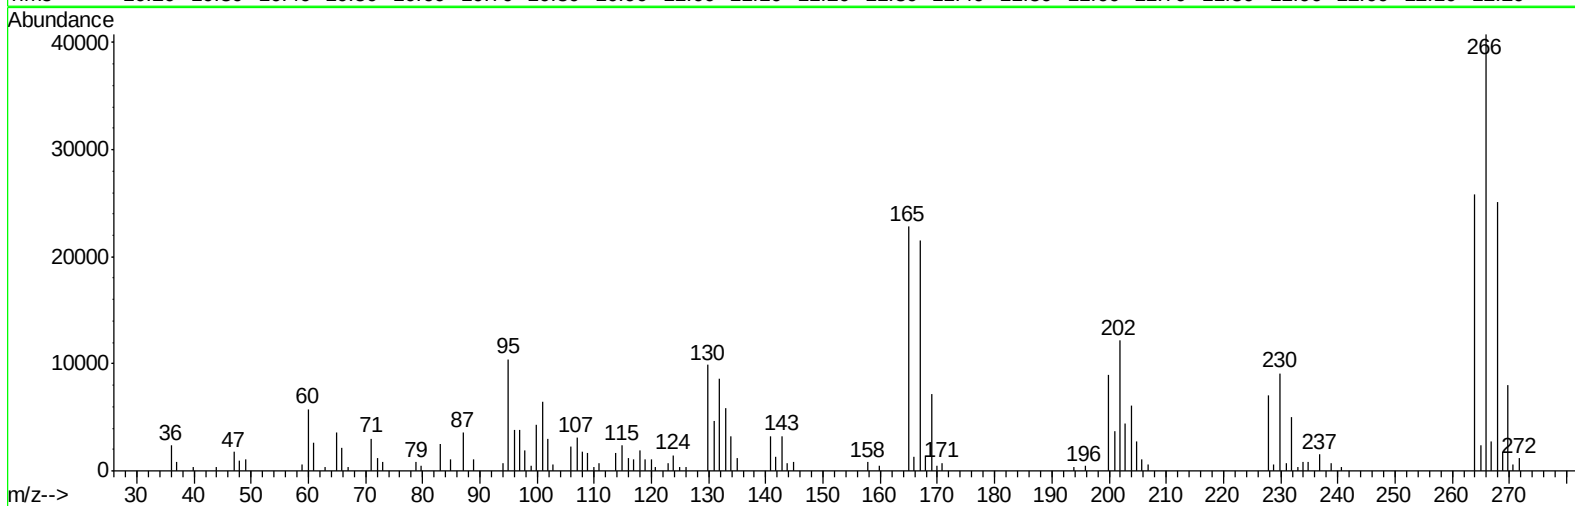


Data Path : Z:\HPCHEM1\BNA F\DATA\BF100817\
Data File : BF099222.D
Acq On : 8 Oct 2017 9:55
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 09 06:49:32 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 05 17:20:48 2017
Response via : Initial Calibration

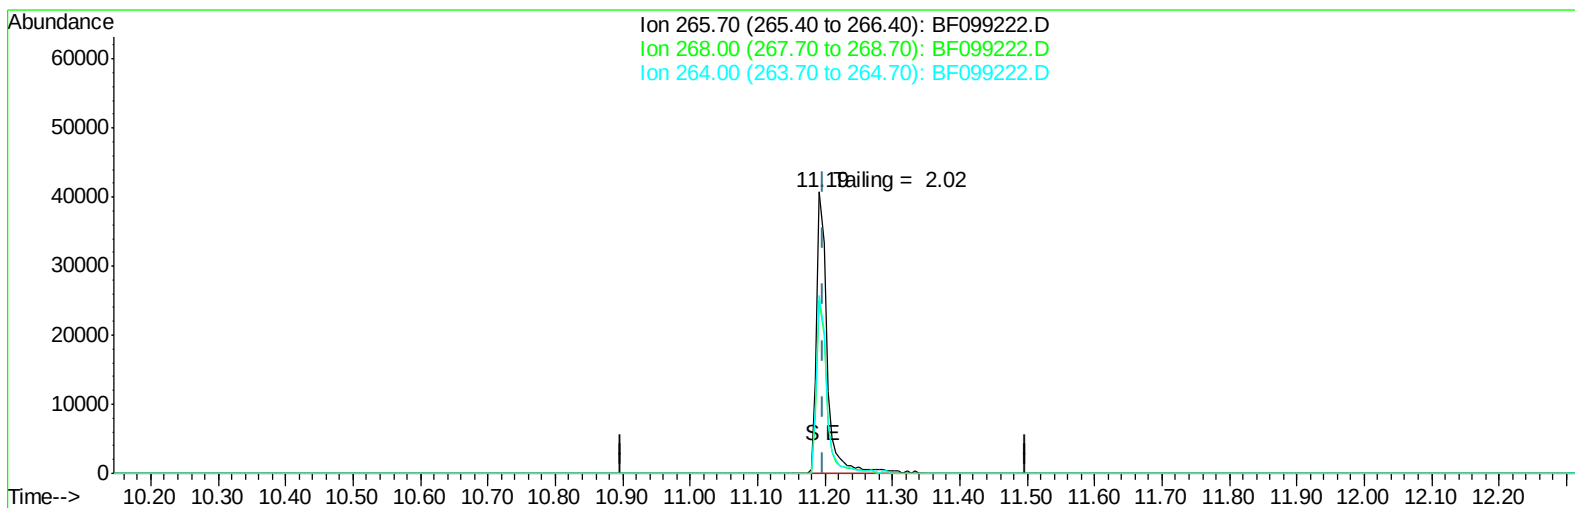

TIC: BF099222.D

(69) Pentachlorophenol (C)



11.192min (-0.006) 37800.13ng

response 42548

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.55
264.00	61.90	63.42
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100817\
Data File : BF099222.D
Acq On : 8 Oct 2017 9:55
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 09 06:49:32 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 05 17:20:48 2017
Response via : Initial Calibration

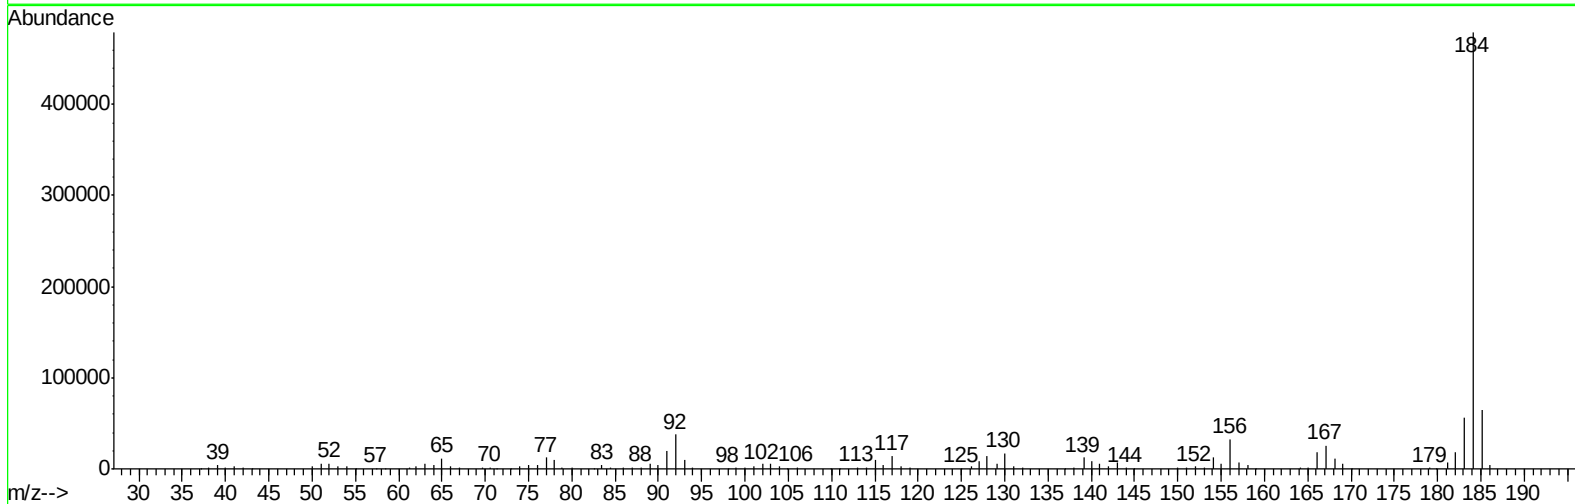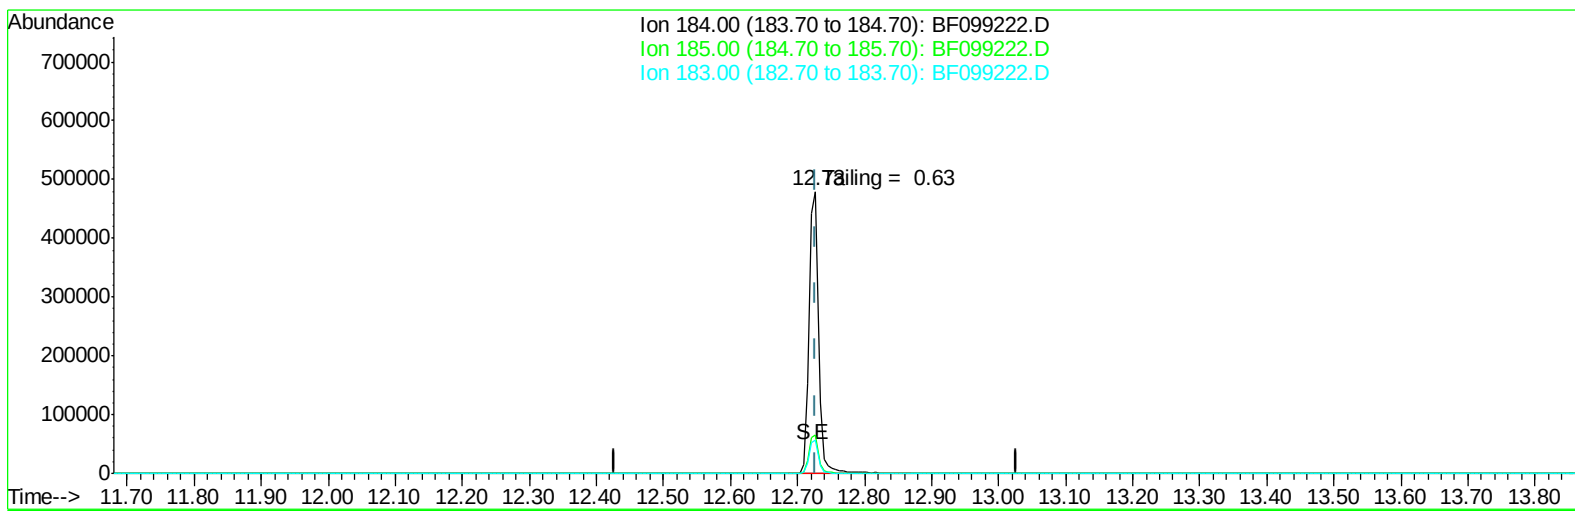

TIC: BF099222.D

(76) Benzidine

12.727min (-0.000) 0.00ng

response 456143

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.51
183.00	11.60	11.73
0.00	0.00	0.00