

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100817\
 Data File : BF099254.D
 Acq On : 9 Oct 2017 2:06
 Operator : SJ/JU
 Sample : I5645-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 100317-TIDO-F-D-B

Quant Time: Oct 09 04:46:02 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 05 17:20:48 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	130670	20.00	ng	0.00
21) Naphthalene-d8	8.15	136	540630	20.00	ng	0.00
38) Acenaphthene-d10	9.90	164	247037	20.00	ng	0.00
63) Phenanthrene-d10	11.39	188	414515	20.00	ng	0.00
75) Chrysene-d12	14.03	240	248400	20.00	ng	0.00
86) Perylene-d12	15.50	264	224983	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.49	112	375842	45.79	ng	0.00
7) Phenol-d6	6.49	99	275271	27.18	ng	0.00
23) Nitrobenzene-d5	7.43	82	808789	95.94	ng	0.00
41) 2,4,6-Tribromophenol	10.69	330	176823	87.47	ng	0.00
44) 2-Fluorobiphenyl	9.22	172	1394875	94.26	ng	0.00
78) Terphenyl-d14	12.97	244	1120770	102.61	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF100817\
Data File : BF099254.D
Acq On : 9 Oct 2017 2:06
Operator : SJ/JU
Sample : I5645-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
100317-TIDO-F-D-B

Quant Time: Oct 09 04:46:02 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 05 17:20:48 2017
Response via : Initial Calibration

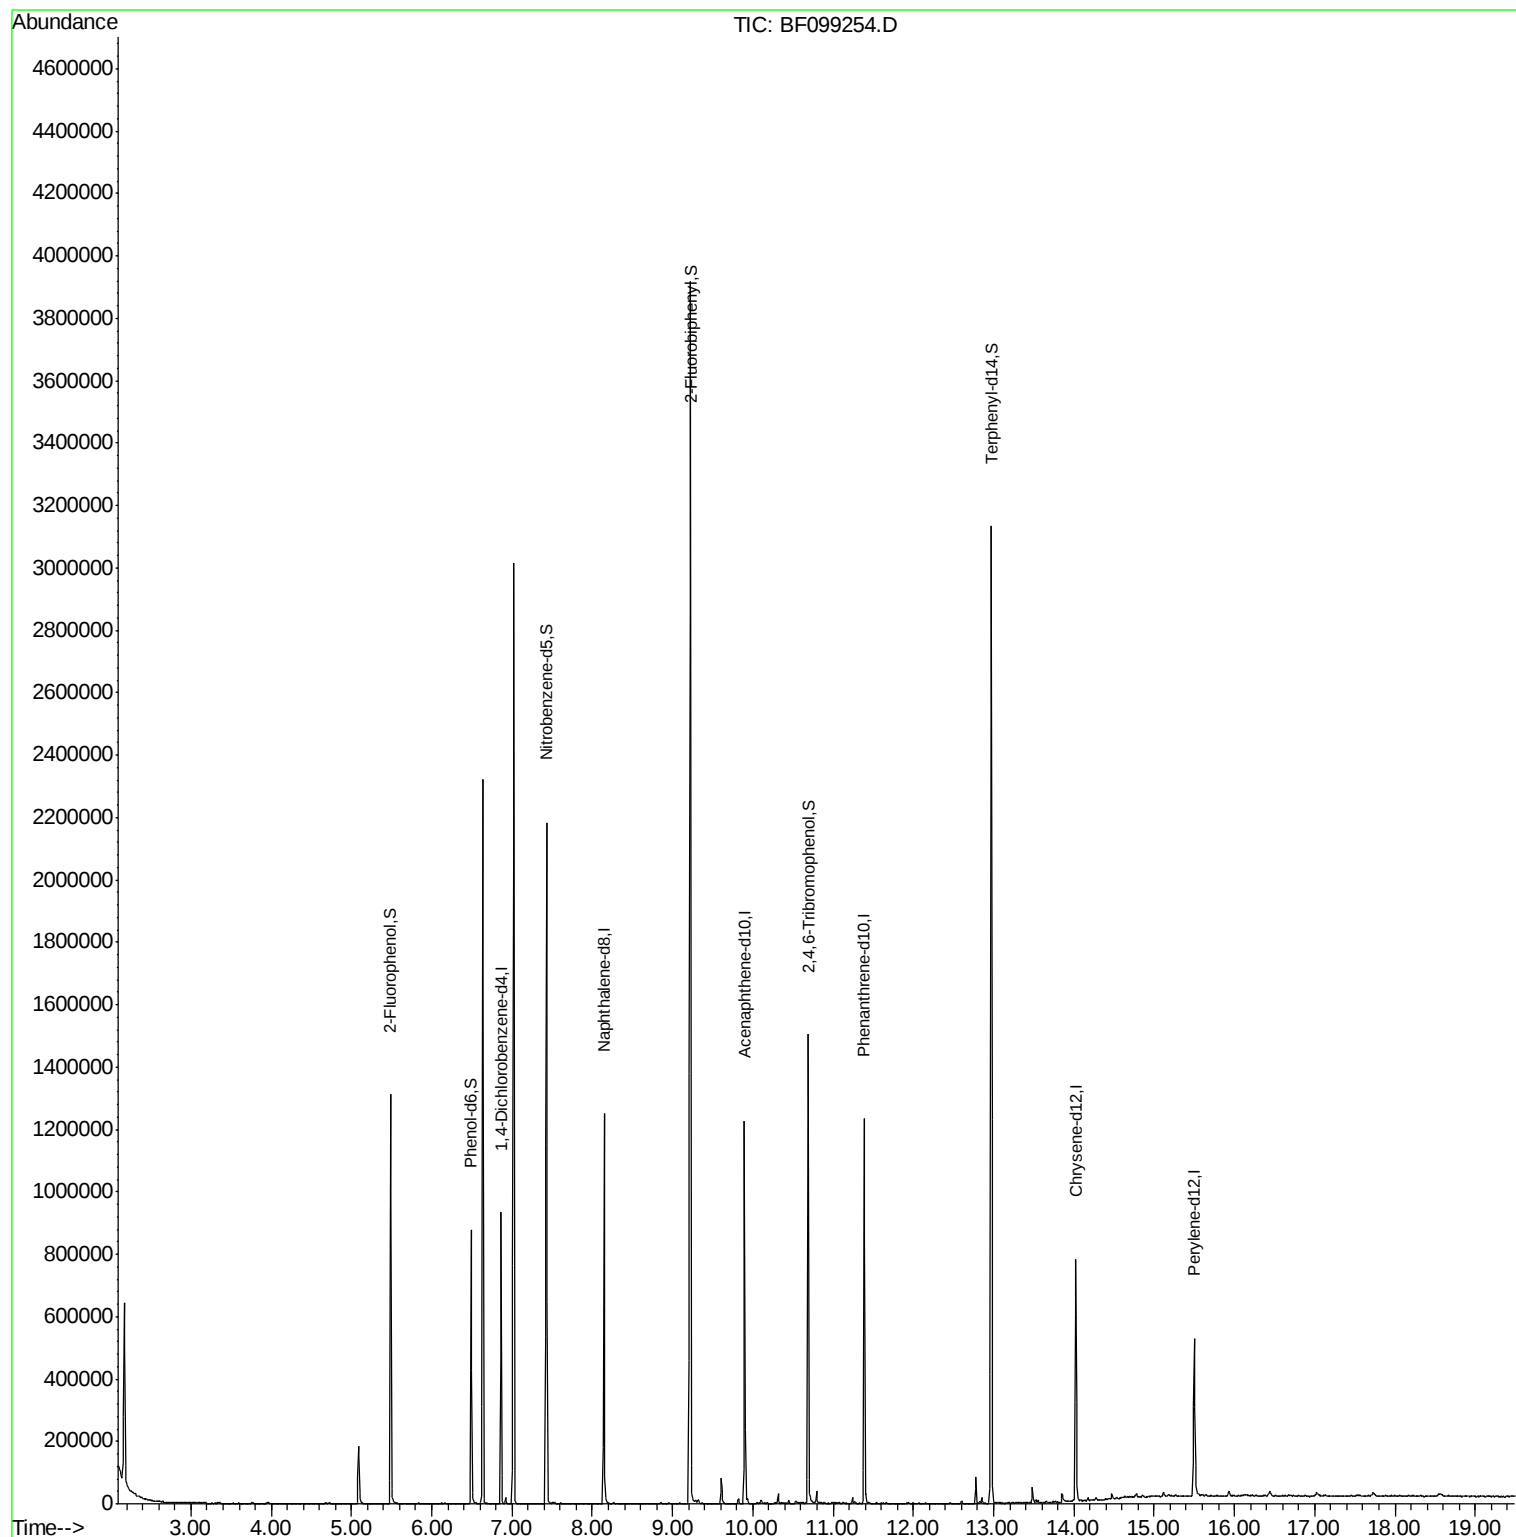




#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.86 min Scan# 812
 Delta R.T. -0.01 min
 Lab File: BF099254.D
 Acq: 9 Oct 2017 2:06

Instrument :
 BNA_F
 ClientSampleId :
 100317-TIDO-F-D-B

Tot Ion:152 Resp: 130670
 Ion Ratio Lower Upper
 152 100
 150 160.5 124.6 186.8
 115 61.3 50.1 75.1

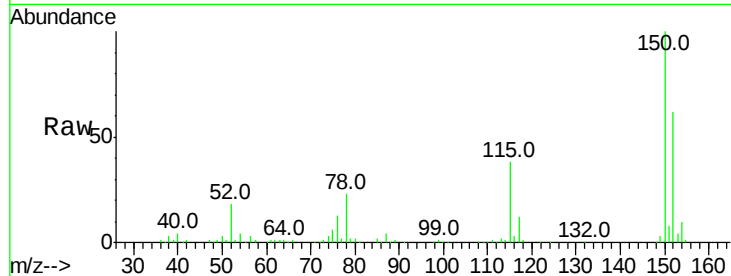


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

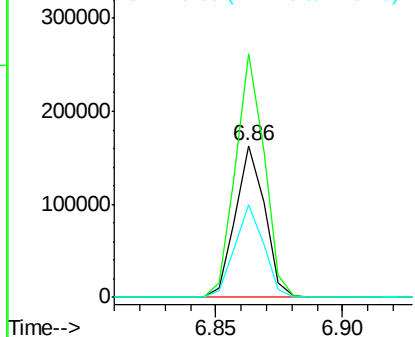



#5

2-Fluorophenol
 Concen: 45.787 ng
 RT: 5.49 min Scan# 578
 Delta R.T. 0.01 min
 Lab File: BF099254.D
 Acq: 9 Oct 2017 2:06

Tgt Ion:112 Resp: 375842
 Ion Ratio Lower Upper
 112 100
 64 56.7 47.9 71.9
 63 26.6 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

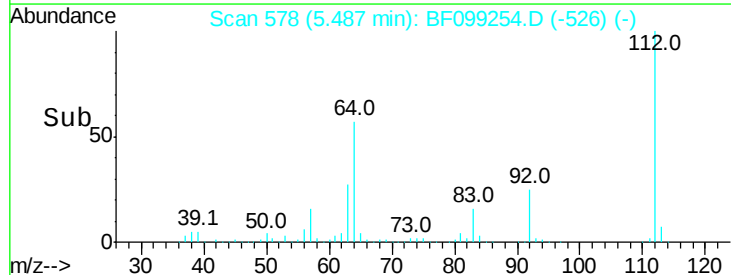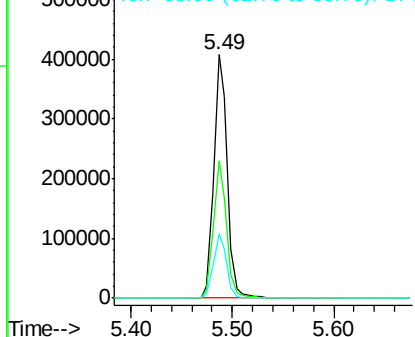



#7

Phenol-d6

Concen: 27.185 ng

RT: 6.49 min Scan# 749

Delta R.T. -0.01 min

Lab File: BF099254.D

Acq: 9 Oct 2017 2:06

Instrument :

BNA_F

ClientSampleId :

100317-TIDO-F-D-B


Tot Ion: 99 Resp: 275271

Ion Ratio Lower Upper

99 100

42 15.4 14.5 21.7



71 30.6 25.4 38.0



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

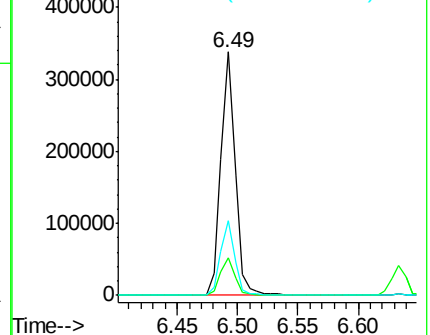

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.15 min Scan# 1030

Delta R.T. -0.01 min

Lab File: BF099254.D

Acq: 9 Oct 2017 2:06

Tgt Ion: 136 Resp: 540630


Ion Ratio Lower Upper

136 100

137 10.9 8.9 13.3

54 7.2 6.6 9.8

68 6.1 5.0 7.4





Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

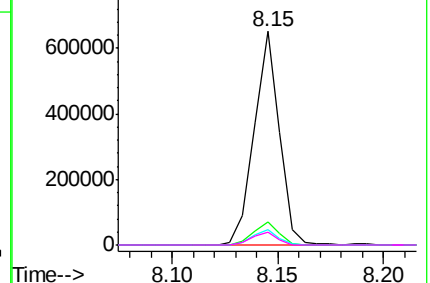







#23
Nitrobenzene-d5
Concen: 95.939 ng
RT: 7.43 min Scan# 909
Delta R.T. -0.00 min
Lab File: BF099254.D
Acq: 9 Oct 2017 2:06

Instrument :
BNA_F
ClientSampleId :
100317-TIDO-F-D-B

Tot Ion: 82 Resp: 808789
Ion Ratio Lower Upper
82 100
128 49.2 36.1 54.1
54 46.8 41.4 62.2

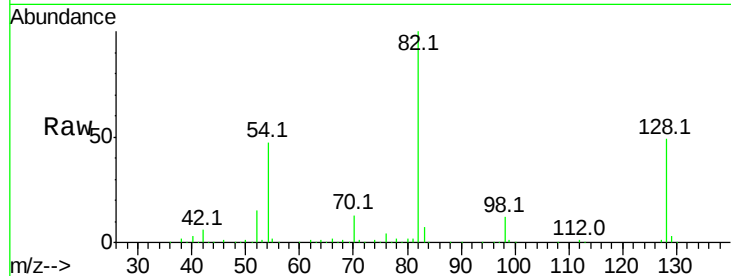


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): B
Ion 54.00 (53.70 to 54.70): BF0


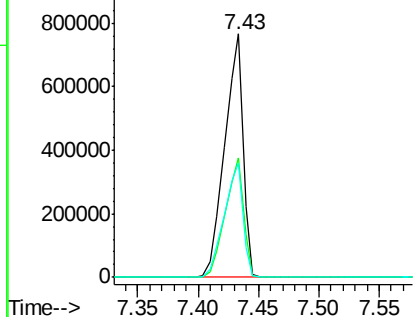


#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.90 min Scan# 1328
Delta R.T. -0.01 min
Lab File: BF099254.D
Acq: 9 Oct 2017 2:06

Tgt Ion:164 Resp: 247037
Ion Ratio Lower Upper
164 100
162 103.0 86.1 129.1
160 44.4 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

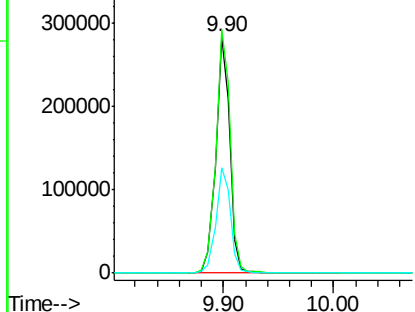







#41
 2,4,6-Tribromophenol
 Concen: 87.474 ng
 RT: 10.69 min Scan# 1463
 Delta R.T. -0.01 min
 Lab File: BF099254.D
 Acq: 9 Oct 2017 2:06

Instrument :
 BNA_F
 ClientSampleId :
 100317-TIDO-F-D-B

Tot Ion:330 Resp: 176823
 Ion Ratio Lower Upper
 330 100
 332 94.6 77.0 115.6
 141 38.7 29.9 44.9

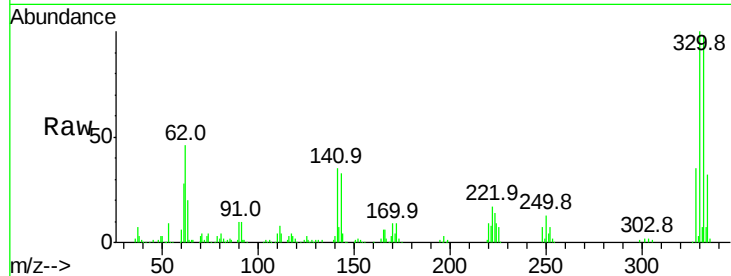


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

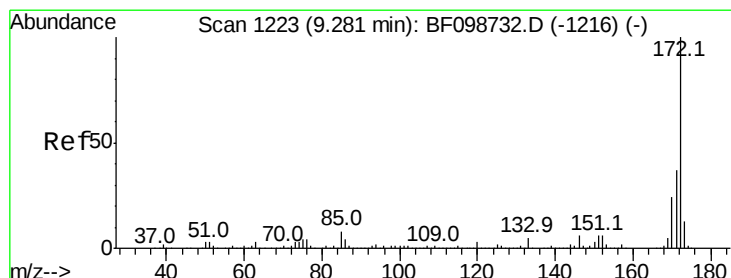
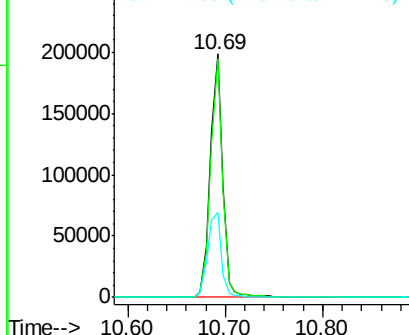



#44
 2-Fluorobiphenyl
 Concen: 94.262 ng
 RT: 9.22 min Scan# 1213
 Delta R.T. -0.01 min
 Lab File: BF099254.D
 Acq: 9 Oct 2017 2:06

Tgt Ion:172 Resp: 1394875
 Ion Ratio Lower Upper
 172 100
 171 36.7 29.7 44.5
 170 23.9 19.6 29.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




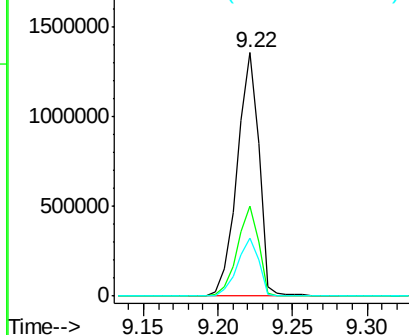


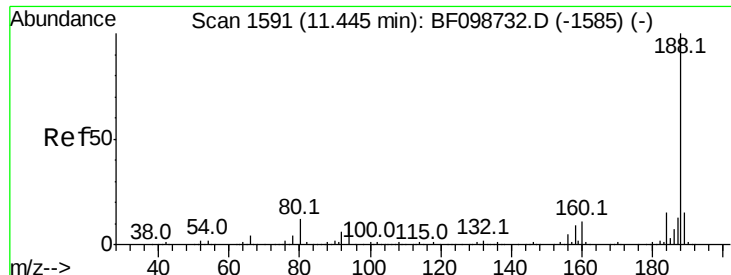

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.39 min Scan# 1581
Delta R.T. -0.01 min
Lab File: BF099254.D
Acq: 9 Oct 2017 2:06




Instrument :
BNA_F
ClientSampleId :
100317-TIDO-F-D-B

Tot Ion:188 Resp: 414515
Ion Ratio Lower Upper
188 100
94 11.0 8.5 12.7
80 12.1 9.2 13.8

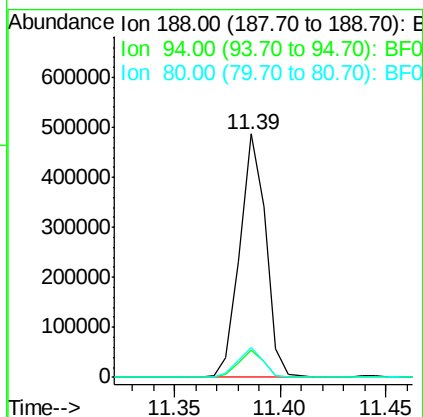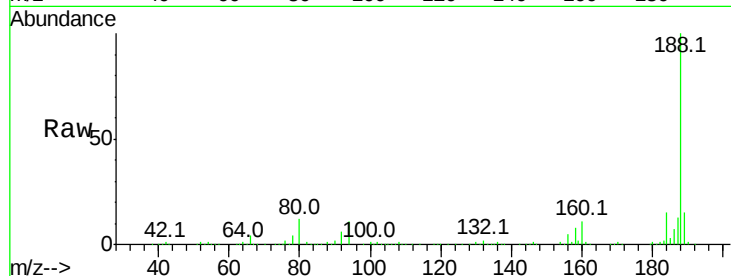

#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.03 min Scan# 2030
Delta R.T. -0.01 min
Lab File: BF099254.D
Acq: 9 Oct 2017 2:06

Tgt Ion:240 Resp: 248400
Ion Ratio Lower Upper
240 100
120 13.8 9.5 14.3
236 25.2 20.7 31.1

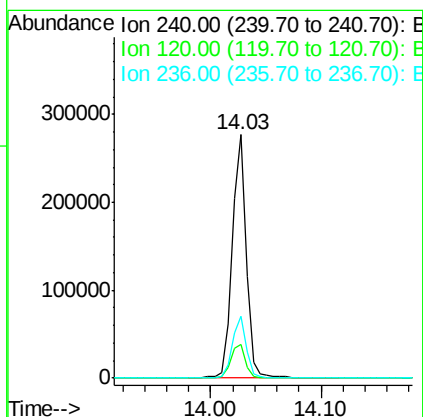



#78

Terphenyl-d14

Concen: 102.611 ng

RT: 12.97 min Scan# 1851

Delta R.T. -0.00 min

Lab File: BF099254.D

Acq: 9 Oct 2017 2:06

Instrument :

BNA_F

ClientSampleId :

100317-TIDO-F-D-B


Tot Ion:244 Resp: 1120770

Ion Ratio Lower Upper

244 100

212 7.0 5.4 8.0




122 13.3 11.0 16.4

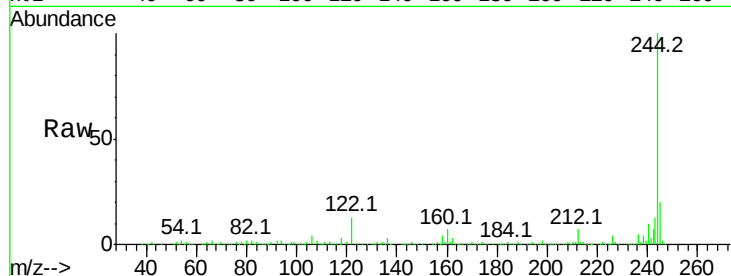

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

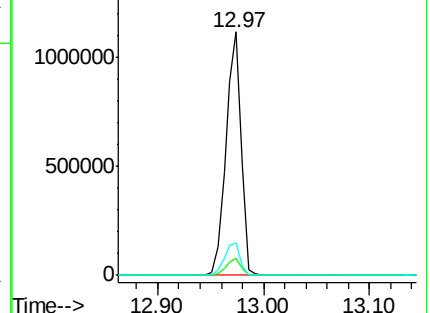

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.50 min Scan# 2281

Delta R.T. -0.00 min

Lab File: BF099254.D

Acq: 9 Oct 2017 2:06


Tgt Ion:264 Resp: 224983

Ion Ratio Lower Upper

264 100

260 23.7 19.2 28.8

265 20.2 17.5 26.3



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

