

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100817\
 Data File : BF099226.D
 Acq On : 8 Oct 2017 12:20
 Operator : SJ/JU
 Sample : PB103045TB
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB103045TB

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.104	509	513	532	rVB	422193	578834	16.31%	1.998%
2	5.498	575	580	583	rBV	2924002	2946764	83.04%	10.170%
3	6.504	745	751	753	rBV	2537223	2886925	81.35%	9.963%
4	6.640	769	774	777	rBV	3075361	3031012	85.41%	10.460%
5	6.863	809	812	816	rBV	946095	766249	21.59%	2.644%
6	7.022	835	839	842	rBV	2685420	2432470	68.55%	8.395%
7	7.428	903	908	911	rBV	1735542	1920162	54.11%	6.627%
8	8.145	1026	1030	1034	rBV	1196118	1059913	29.87%	3.658%
9	9.222	1207	1213	1216	rBV	3556866	3548601	100.00%	12.247%
10	9.904	1323	1329	1332	rBV	1169488	1170721	32.99%	4.040%
11	10.692	1458	1463	1475	rBV	1861516	1918863	54.07%	6.622%
12	11.386	1577	1581	1585	rBV	1238196	1188698	33.50%	4.102%
13	12.780	1815	1818	1822	rBV	200693	150565	4.24%	0.520%
14	12.974	1846	1851	1854	rBV	3078471	3353691	94.51%	11.574%
15	13.486	1934	1938	1941	rBV	143223	109869	3.10%	0.379%
16	14.027	2026	2030	2034	rBV	1192100	1067493	30.08%	3.684%
17	15.504	2276	2281	2289	rBV	643756	845130	23.82%	2.917%


Sum of corrected areas: 28975960

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF100817\
Data File : BF099226.D
Acq On : 8 Oct 2017 12:20
Operator : SJ/JU
Sample : PB103045TB
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB103045TB

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

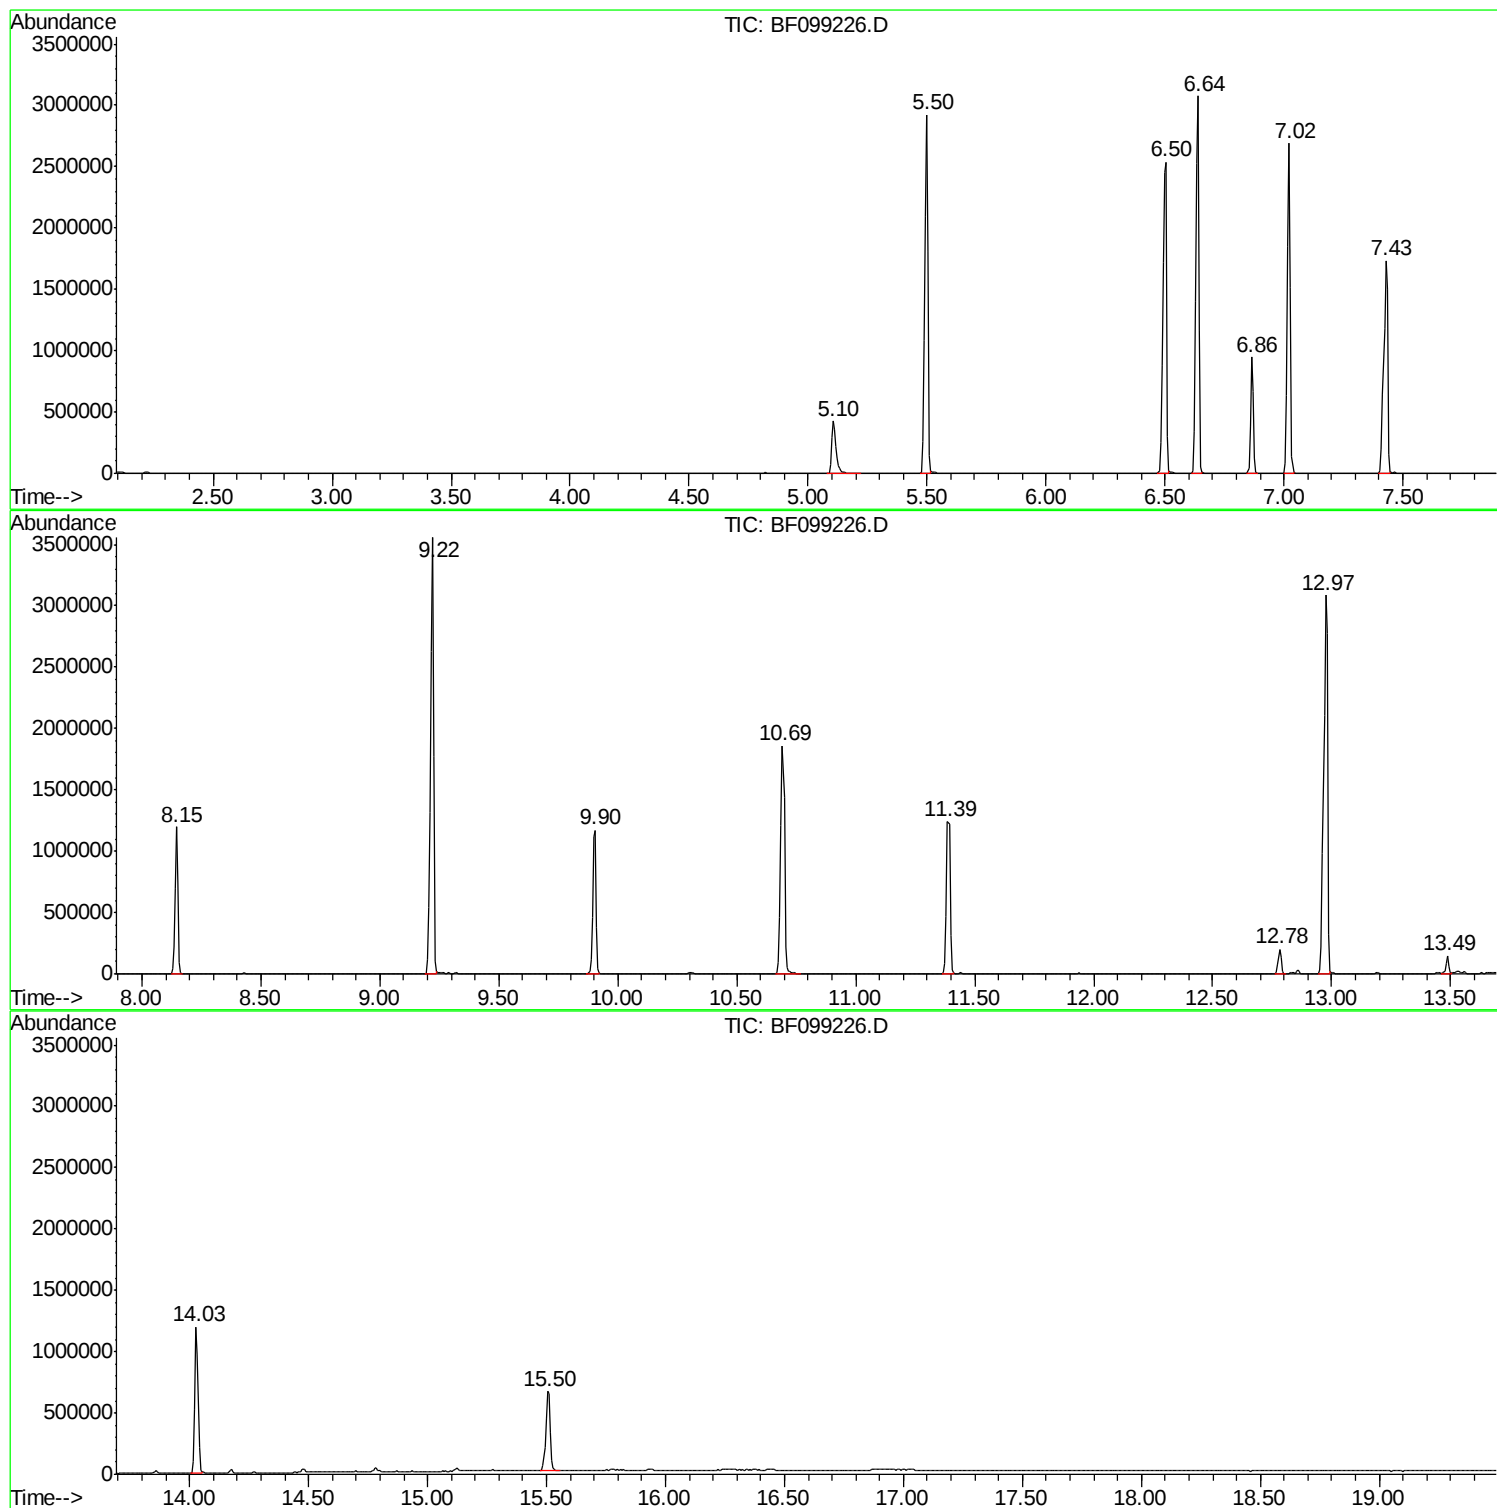

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF100817\
Data_File : BF099226.D
Acq_On : 8_Oct_2017. 12:200
Operator : SJ/JUU
Sample : PB103045TBB
Misc :
ALS_Vial : 5 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
PB103045TB

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
