


Data Path : Z:\HPCHEM1\BNA F\Data\BF100817\
 Data File : BF099247.D
 Acq On : 8 Oct 2017 22:47
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 05 17:20:48 2017

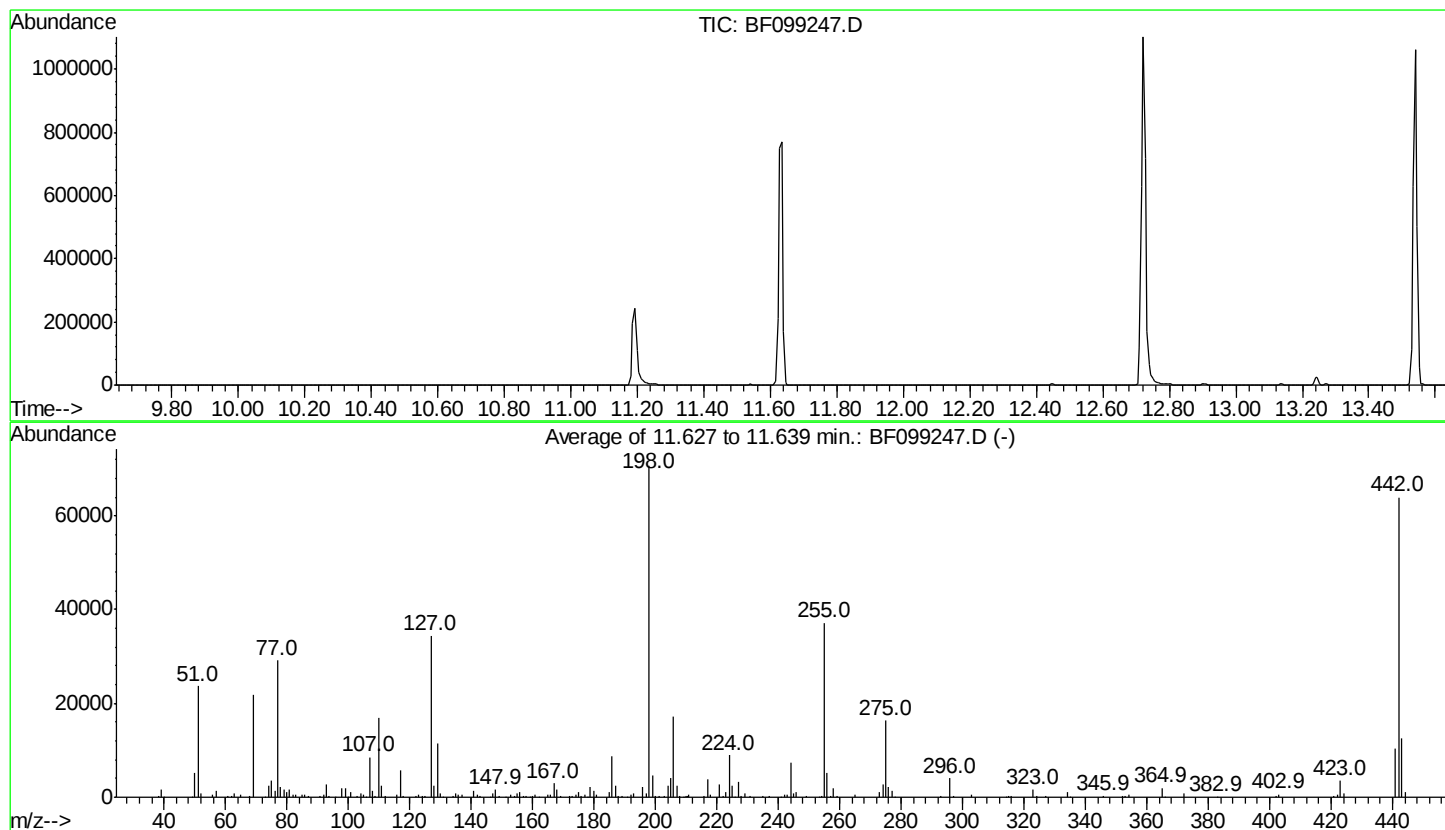

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	23686	PASS
68	69	0.00	2	1.6	350	PASS
69	198	0.00	100	30.8	21808	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.7	34419	PASS
197	198	0.00	2	1.0	720	PASS
198	198	100	100	100.0	70714	PASS
199	198	5	9	6.7	4711	PASS
275	198	10	60	23.0	16263	PASS
365	198	1	100	2.8	1988	PASS
441	442	0.01	24	16.3	10424	PASS
442	198	50	100	90.4	63960	PASS
443	442	15	24	19.8	12646	PASS