


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF100818\
 Data File : BF109641.D
 Acq On : 8 Oct 2018 12:03
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF100818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 08 16:02:11 2018

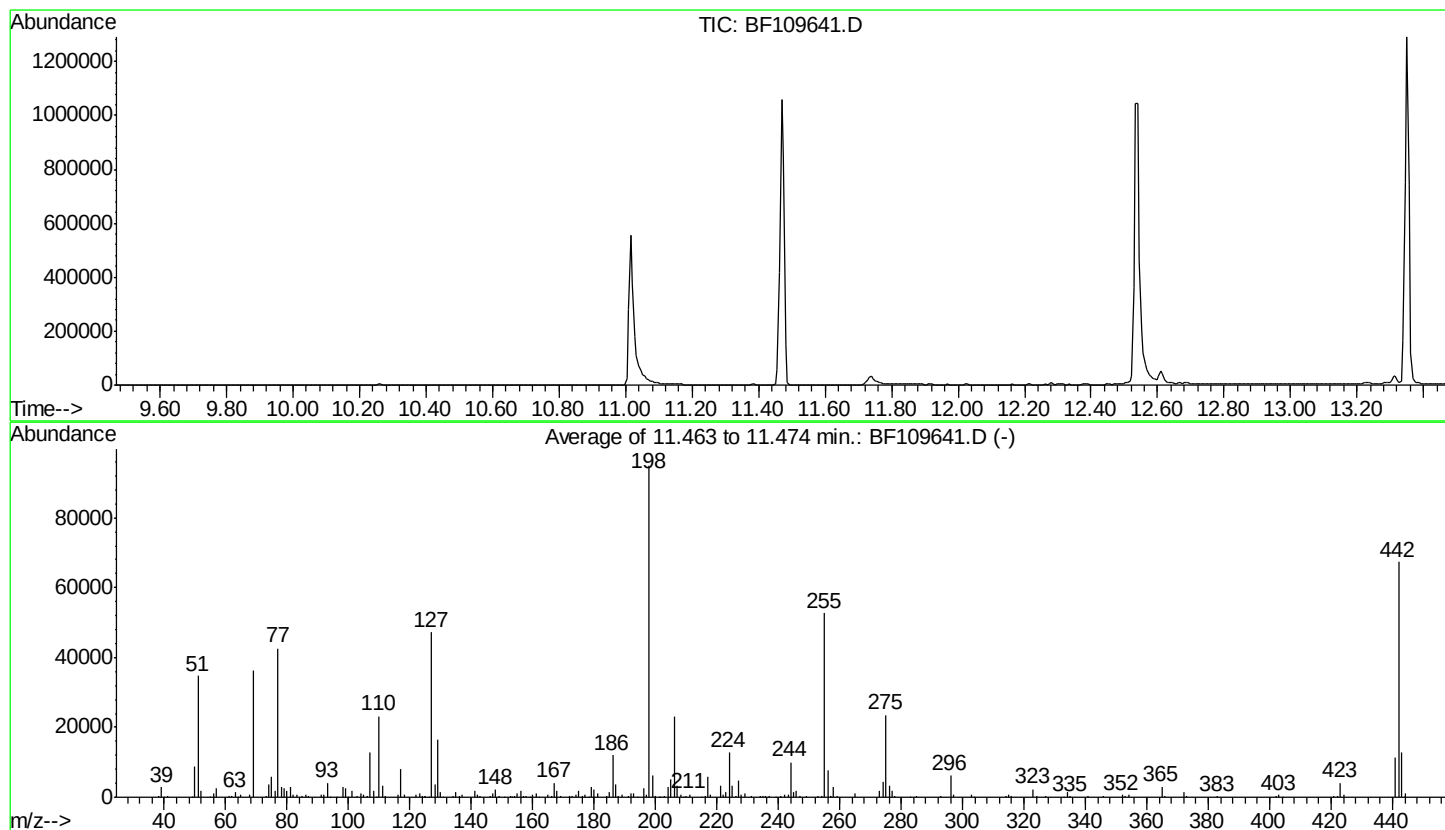

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	34720	PASS
68	69	0.00	2	1.7	599	PASS
69	198	0.00	100	38.2	36226	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.7	47224	PASS
197	198	0.00	2	0.7	653	PASS
198	198	100	100	100.0	94944	PASS
199	198	5	9	6.5	6205	PASS
275	198	10	60	24.9	23598	PASS
365	198	1	100	3.1	2962	PASS
441	198	0.01	100	11.9	11323	PASS
442	198	50	100	71.0	67408	PASS
443	442	15	24	19.0	12819	PASS